
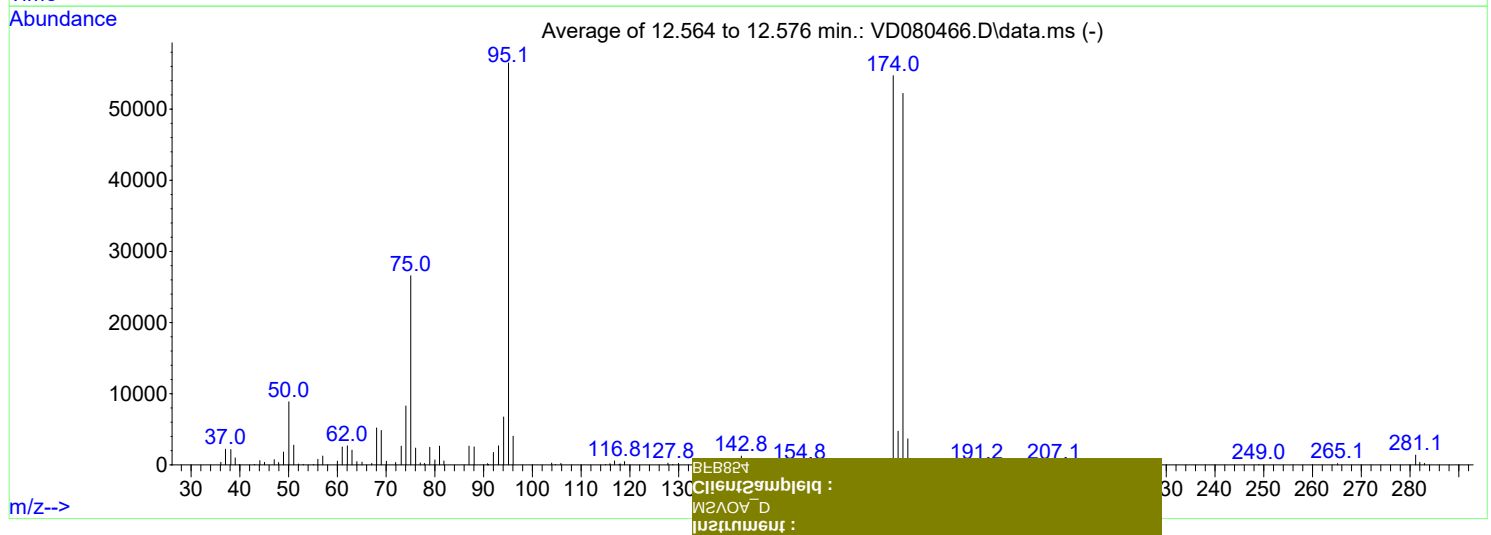


Data Path : D:\MassHunter\GCMS\1\data\VD062325\
Data File : VD080466.D
Acq On : 23 Jun 2025 08:30
Operator : RP/MD
Sample : BFB854
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061825SMA.M
Title : SFAM01.0
Last Update : Mon Jun 23 08:51:45 2025

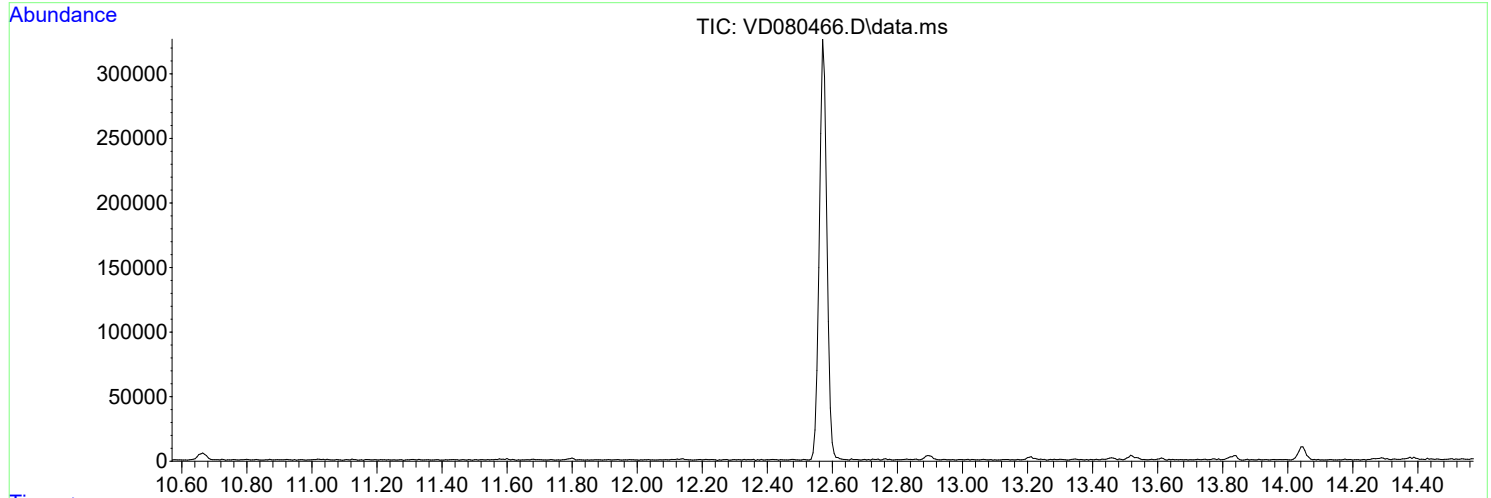

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1828

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	8871	PASS
75	95	30	80	47.1	26587	PASS
95	95	100	100	100.0	56501	PASS
96	95	5	9	7.1	4038	PASS
173	174	0.00	2	1.3	710	PASS
174	95	50	120	96.8	54709	PASS
175	174	5	9	8.7	4741	PASS
176	174	95	105	95.4	52216	PASS
177	176	5	10	7.0	3661	PASS

m/z	Abundance
39.90	746.0
43.80	291.0

BFB824
Client Sample :
MSA04.D
Instrument :

m/z	Abundance
36.20	254.0
37.10	1914.0
38.20	2298.0
39.10	933.0
40.00	899.0
44.20	555.0
45.00	369.0
47.00	916.0
48.00	272.0
48.90	1301.0
50.00	8500.0
51.00	2719.0
56.10	599.0
56.90	1218.0
60.10	599.0
61.00	2167.0
62.10	2266.0
63.00	1808.0
63.90	415.0
65.00	258.0
67.00	327.0
68.10	4091.0
69.00	3863.0
70.10	622.0
72.10	253.0
73.10	2133.0
74.10	6995.0
75.10	23080.0
76.00	1869.0
78.90	2309.0
80.00	451.0
80.90	2609.0
81.80	491.0
87.00	2496.0
88.00	2269.0
90.80	187.0
92.00	1436.0
93.10	2394.0
94.10	5219.0
95.10	48832.0
96.10	4036.0
103.90	287.0
105.90	209.0
115.00	151.0
115.90	287.0
116.90	410.0
117.80	245.0
119.00	396.0
127.80	313.0
130.00	188.0
133.10	189.0
140.90	506.0
142.80	1064.0
144.60	321.0
145.00	444.0
145.90	212.0
154.70	151.0
171.10	285.0
172.00	249.0
173.00	679.0
174.00	47880.0
175.00	4347.0
176.00	44640.0
177.00	2760.0
191.20	152.0
281.30	898.0
282.00	234.0

BFB824
Client Sample ID :
MS/MS.D
Instrument :

m/z	Abundance
36.10	512.0
37.00	2506.0
38.10	2638.0
39.10	1007.0
40.00	684.0
43.00	175.0
44.00	819.0
45.10	424.0
47.10	731.0
47.90	402.0
49.00	1841.0
50.10	9582.0
51.00	2728.0
52.00	169.0
55.90	768.0
57.00	1377.0
60.00	496.0
61.00	2695.0
62.00	3272.0
63.00	2236.0
64.00	408.0
65.00	489.0
67.10	280.0
68.00	5872.0
69.00	5262.0
70.10	428.0
71.90	390.0
73.10	3403.0
74.10	9502.0
75.00	30088.0
76.00	3248.0
77.10	513.0
77.90	301.0
79.00	2651.0
79.80	509.0
80.10	483.0
80.90	2654.0
81.80	664.0
87.00	3279.0
88.00	3261.0
90.80	338.0
92.00	1972.0
93.00	3081.0
94.10	7766.0
95.10	63128.0
96.10	4526.0
103.90	231.0
104.70	160.0
105.90	235.0
115.90	226.0
116.90	682.0
118.00	243.0
118.80	406.0
127.80	301.0
129.90	321.0
140.80	561.0
142.90	1273.0
144.90	329.0
147.80	228.0
156.80	164.0
160.90	162.0
171.00	412.0
172.10	355.0
173.10	1451.0
174.00	58536.0
175.00	5529.0
176.00	57920.0
177.00	4272.0
190.80	250.0
206.90	171.0
249.00	189.0
265.10	194.0
281.10	1836.0
282.00	393.0
283.00	280.0

BFB854
ClientSampleId :
MS/MS.D
Instrument :

m/z	Abundance
36.00	338.0
37.00	2198.0
38.10	1535.0
39.00	994.0
40.00	818.0
44.00	444.0
45.10	259.0
47.00	536.0
47.90	337.0
49.00	2270.0
50.10	8530.0
51.10	2870.0
52.10	200.0
53.00	195.0
55.10	180.0
56.00	981.0
57.10	1145.0
59.90	502.0
61.00	2679.0
62.00	2501.0
63.00	2187.0
64.10	586.0
65.10	410.0
68.00	5622.0
69.00	5403.0
70.00	479.0
71.80	367.0
73.10	2356.0
74.00	8363.0
75.00	26592.0
76.10	1980.0
76.90	316.0
77.80	344.0
78.90	2462.0
80.10	689.0
81.00	2649.0
81.90	527.0
87.00	2132.0
88.10	2066.0
91.00	243.0
92.00	1831.0
93.00	2562.0
94.10	7210.0
95.10	57544.0
96.00	3553.0
104.00	233.0
105.80	187.0
116.80	583.0
118.00	191.0
118.90	605.0
127.90	156.0
128.80	153.0
129.90	150.0
140.90	610.0
142.90	1370.0
144.90	574.0
154.80	210.0
161.00	162.0
170.90	216.0
171.80	392.0
174.00	57712.0
175.00	4346.0
176.00	54088.0
177.00	3952.0
191.20	176.0
192.90	252.0
207.10	311.0
265.20	369.0
281.10	1424.0
282.00	467.0
282.90	343.0

BFB824
Client Sample ID :
MS/MS.D
Instrument :