
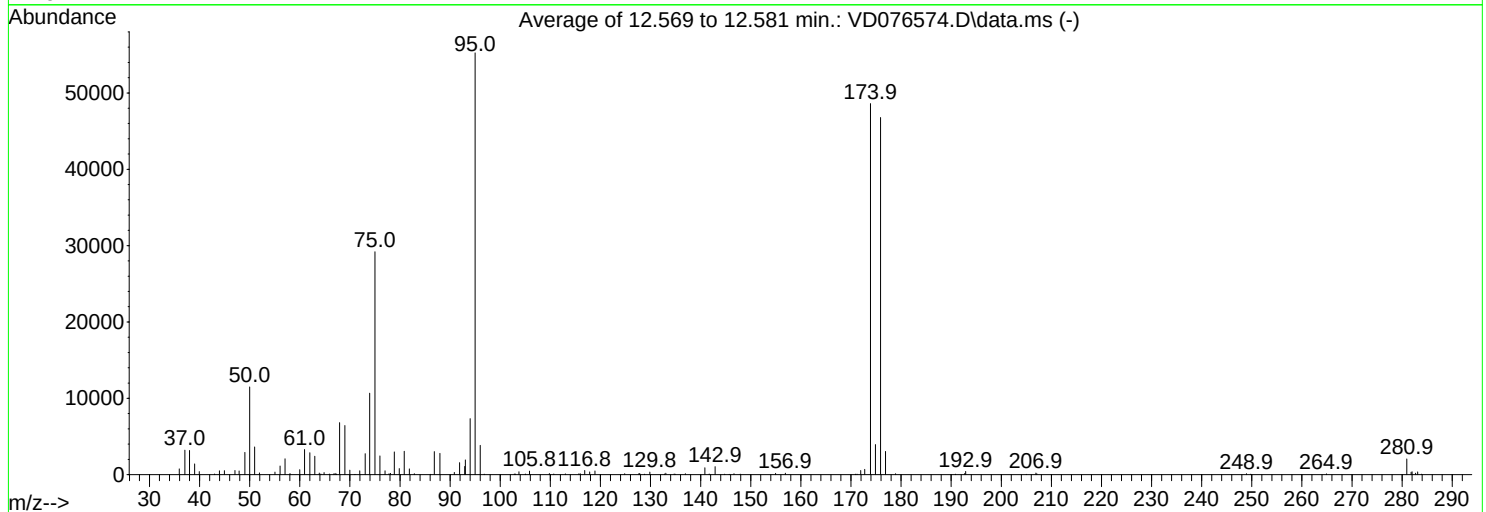


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062623\
 Data File : VD076574.D
 Acq On : 26 Jun 2023 09:07
 Operator : KP/SY
 Sample : BFB
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Title : SW846 8260
 Last Update : Mon Jun 19 04:51:45 2023

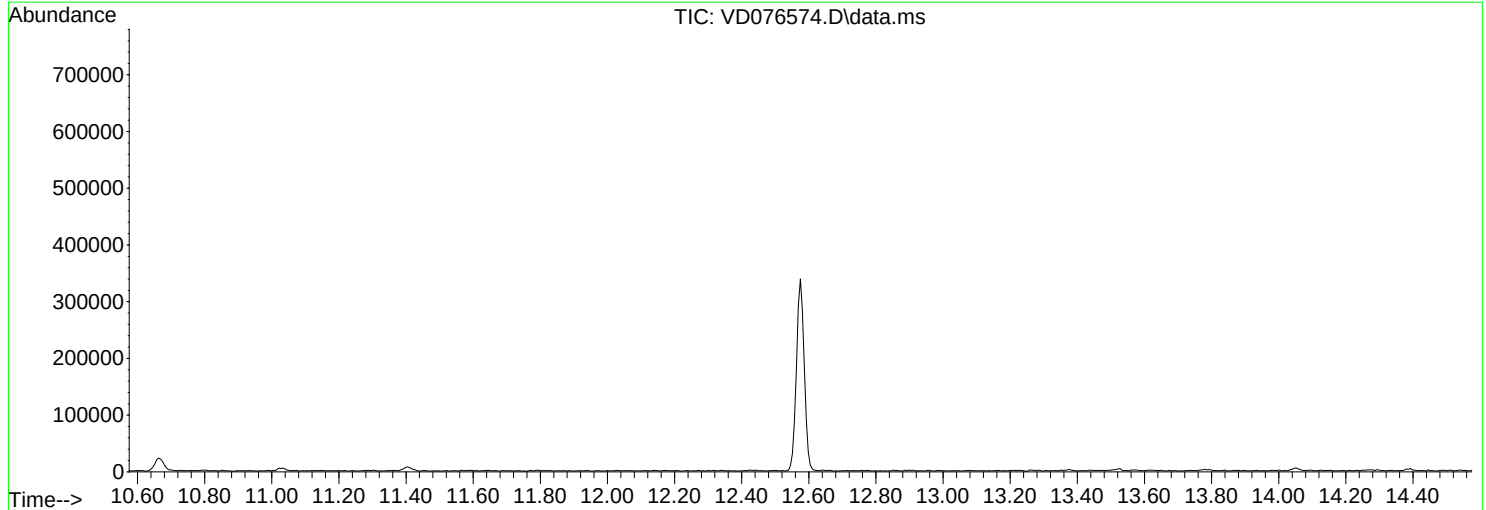

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	11486	PASS
75	95	30	60	52.8	29195	PASS
95	95	100	100	100.0	55256	PASS
96	95	5	9	6.9	3826	PASS
173	174	0.00	2	1.4	685	PASS
174	95	50	100	88.0	48603	PASS
175	174	5	9	8.1	3932	PASS
176	174	95	101	96.3	46781	PASS
177	176	5	9	6.5	3044	PASS