
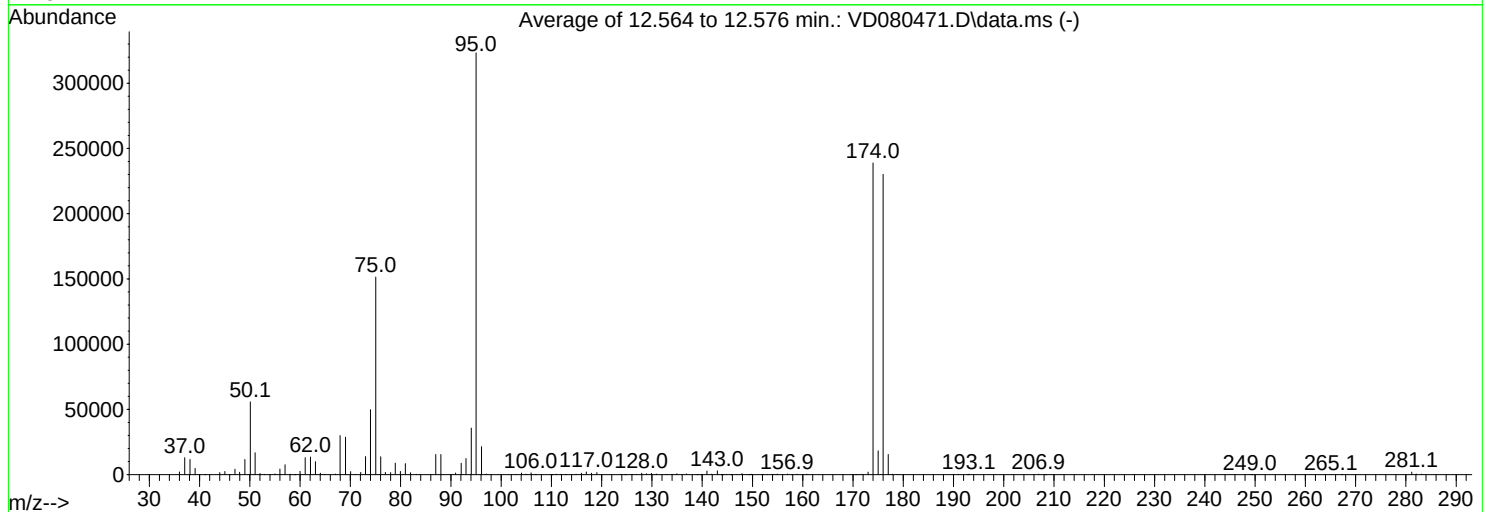


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062625\
Data File : VD080471.D
Acq On : 26 Jun 2025 08:52
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062625S.M
Title : SW846 8260
Last Update : Fri Jun 27 05:16:36 2025

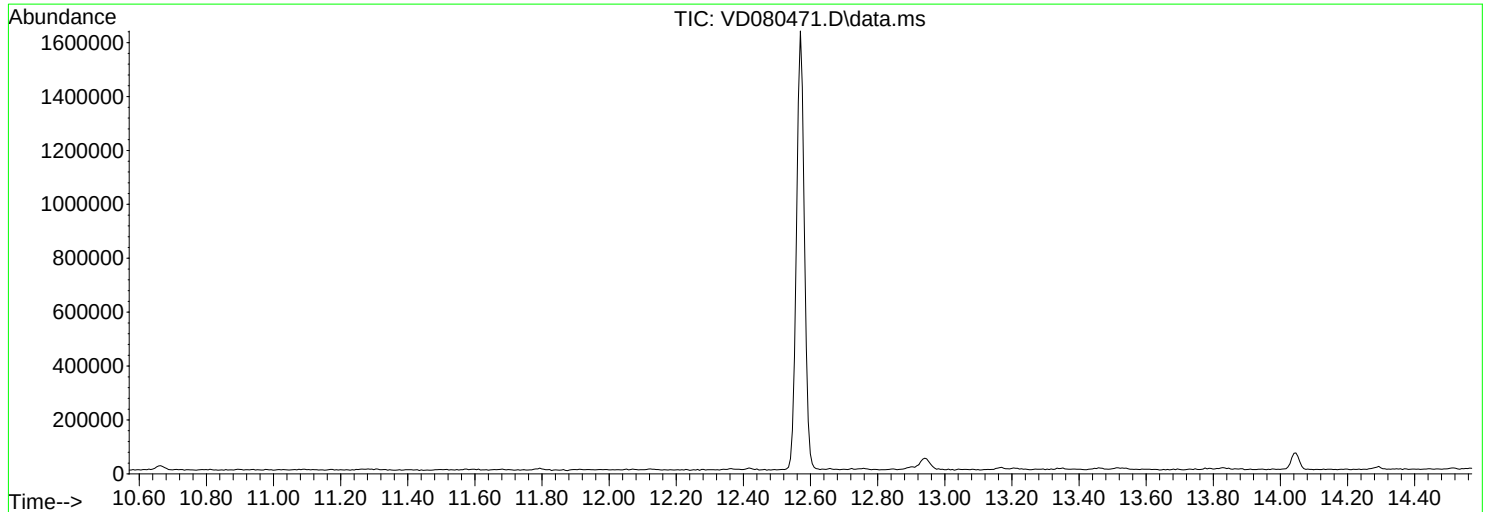

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1823

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	55768	PASS
75	95	30	60	46.8	151445	PASS
95	95	100	100	100.0	323285	PASS
96	95	5	9	6.6	21421	PASS
173	174	0.00	2	0.8	2028	PASS
174	95	50	100	73.9	238848	PASS
175	174	5	9	7.6	18261	PASS
176	174	95	101	96.4	230187	PASS
177	176	5	9	6.7	15487	PASS