
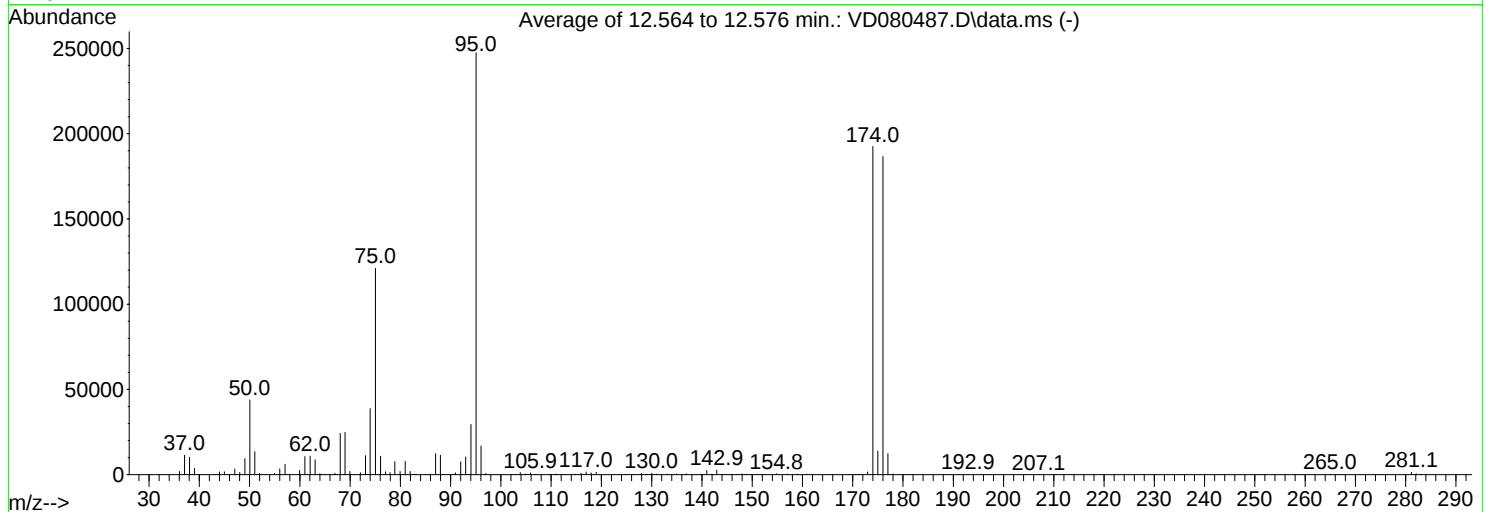


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062725\
Data File : VD080487.D
Acq On : 27 Jun 2025 08:32
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062625S.M
Title : SW846 8260
Last Update : Fri Jun 27 05:16:36 2025

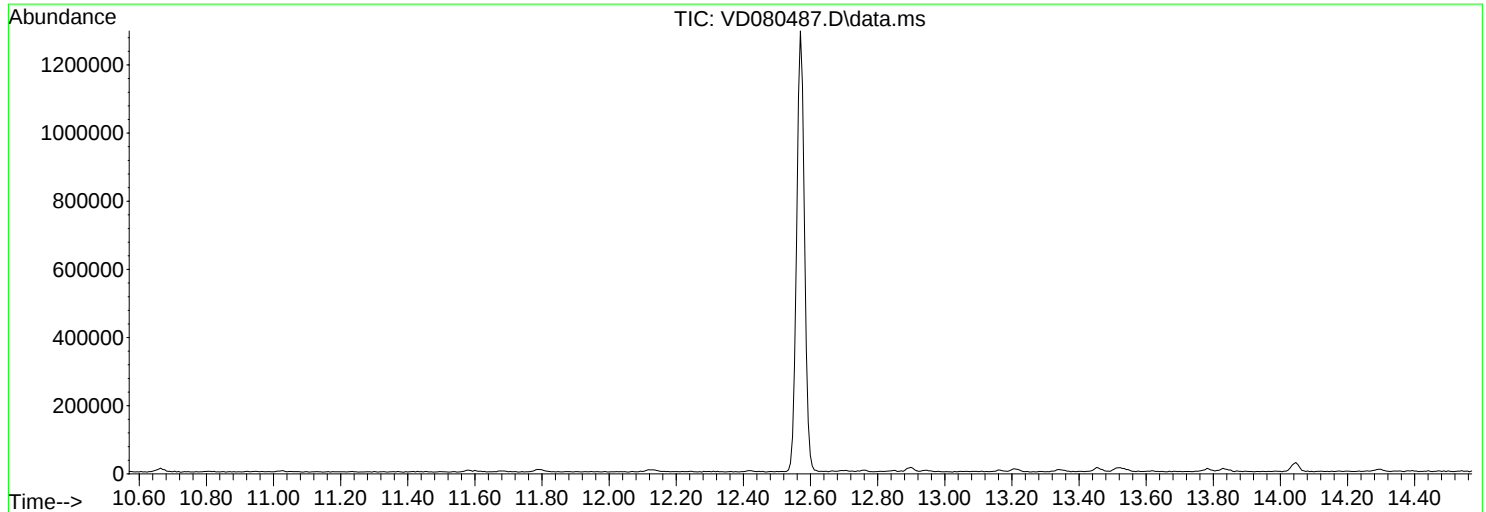

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	43805	PASS
75	95	30	60	48.9	121048	PASS
95	95	100	100	100.0	247467	PASS
96	95	5	9	6.8	16814	PASS
173	174	0.00	2	0.8	1602	PASS
174	95	50	100	77.8	192533	PASS
175	174	5	9	7.2	13832	PASS
176	174	95	101	96.9	186624	PASS
177	176	5	9	6.6	12260	PASS