


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD070219\
 Data File : VD062999.D
 Acq On : 2 Jul 2019 9:45
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
 Title : SW846 8260
 Last Update : Thu Jun 20 01:50:56 2019

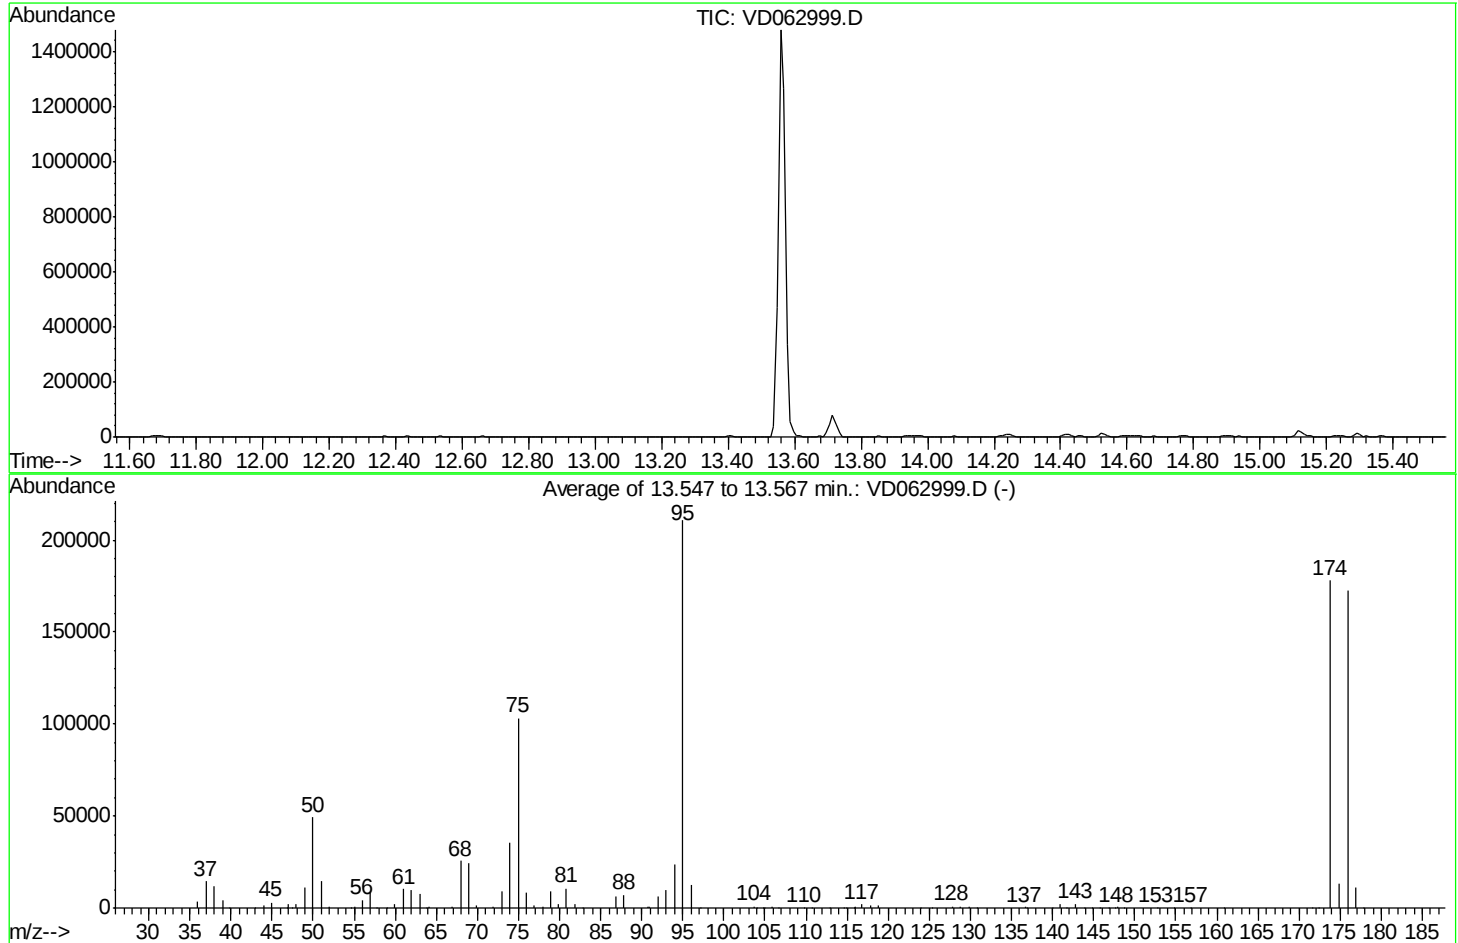

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1227

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	49173	PASS
75	95	30	60	49.0	103186	PASS
95	95	100	100	100.0	210776	PASS
96	95	5	9	6.1	12900	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.4	177920	PASS
175	174	5	9	7.3	12908	PASS
176	174	95	101	97.0	172653	PASS
177	176	5	9	6.3	10904	PASS