
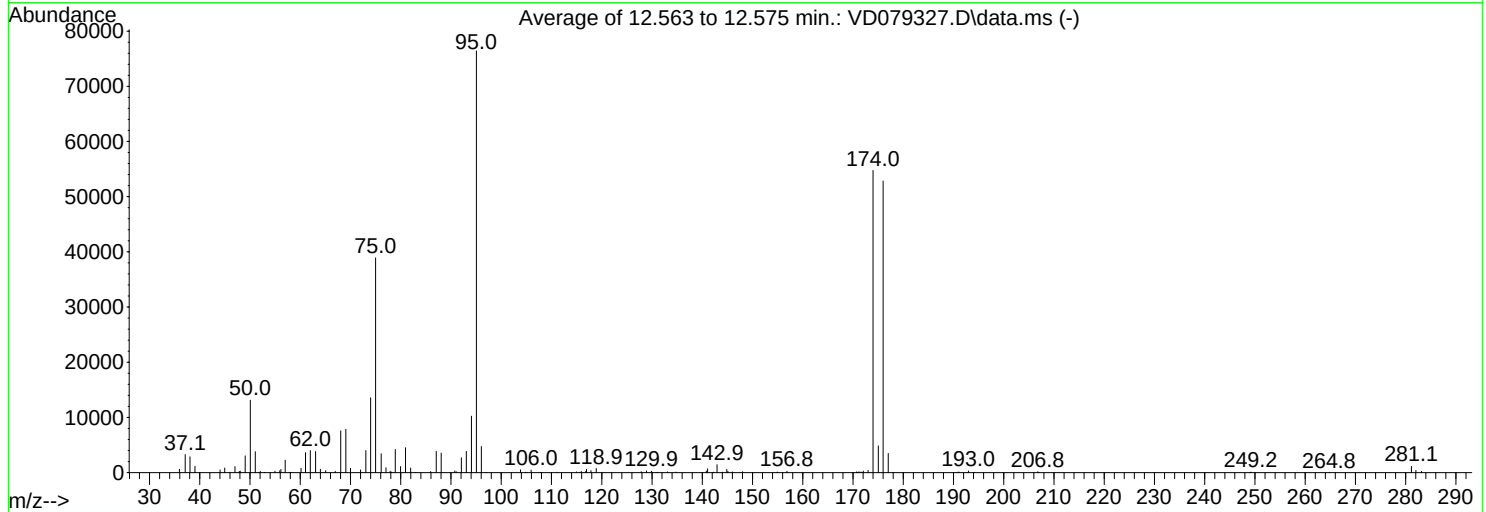


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070324\
Data File : VD079327.D
Acq On : 03 Jul 2024 09:23
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062824S.M
Title : SW846 8260
Last Update : Sat Jun 29 06:28:31 2024

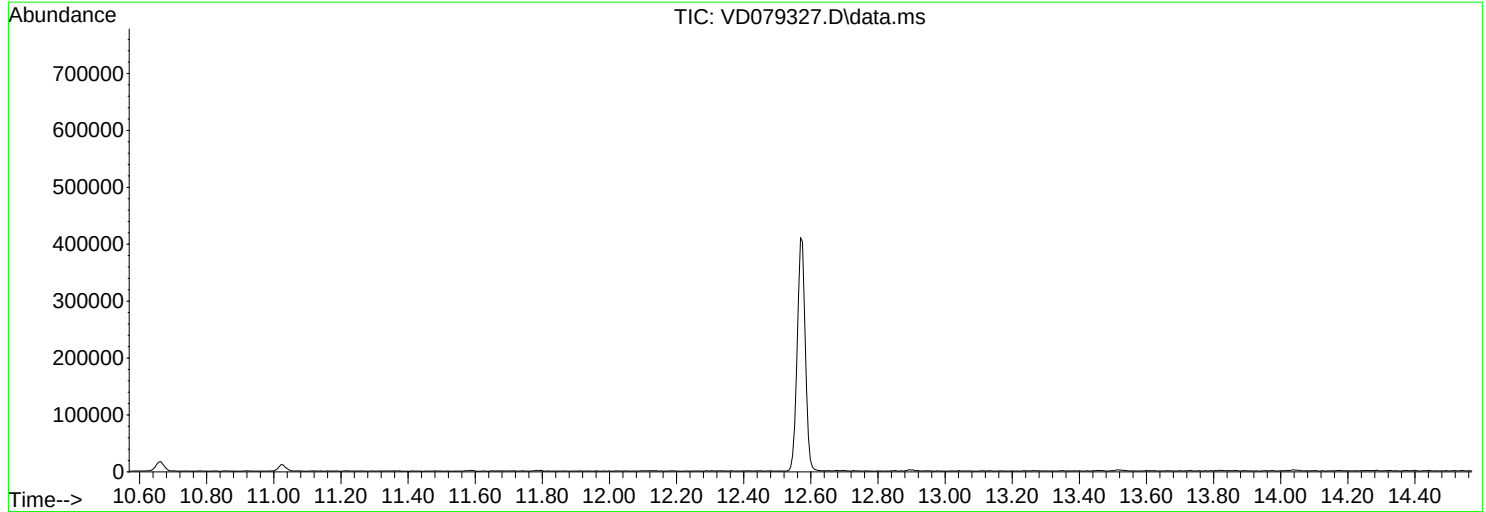

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	13140	PASS
75	95	30	60	50.9	38917	PASS
95	95	100	100	100.0	76427	PASS
96	95	5	9	6.2	4713	PASS
173	174	0.00	2	0.7	408	PASS
174	95	50	100	71.6	54752	PASS
175	174	5	9	8.9	4857	PASS
176	174	95	101	96.5	52845	PASS
177	176	5	9	6.6	3492	PASS