
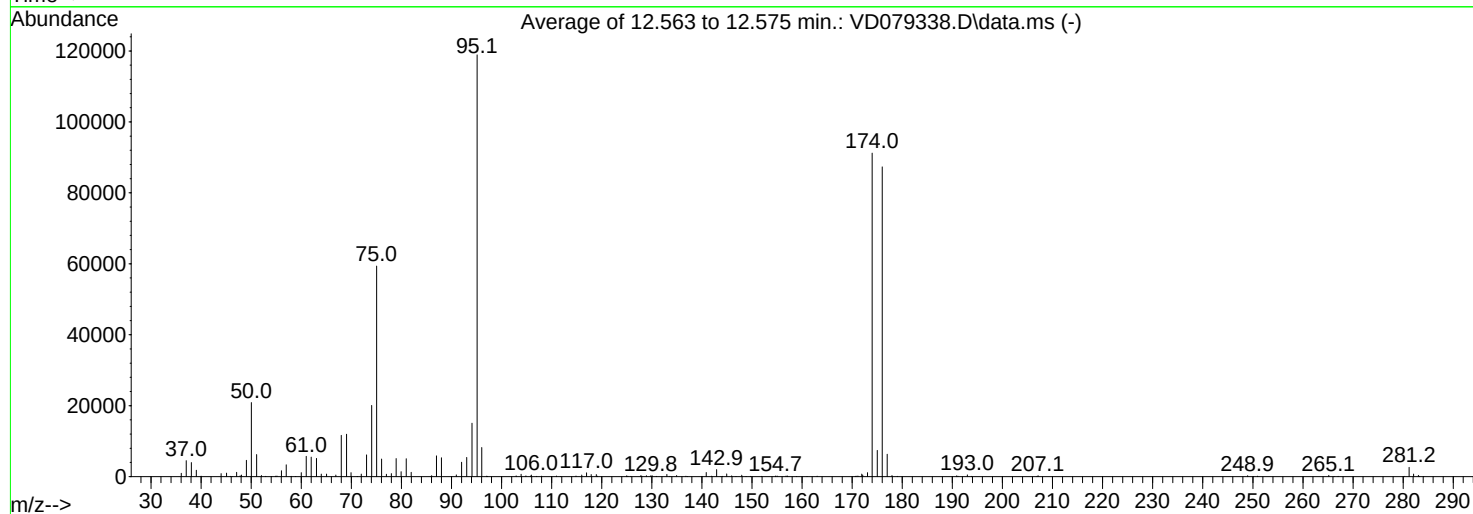


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070824\
Data File : VD079338.D
Acq On : 08 Jul 2024 12:50
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D070824S.M
Title : SW846 8260
Last Update : Mon Jul 08 17:06:59 2024

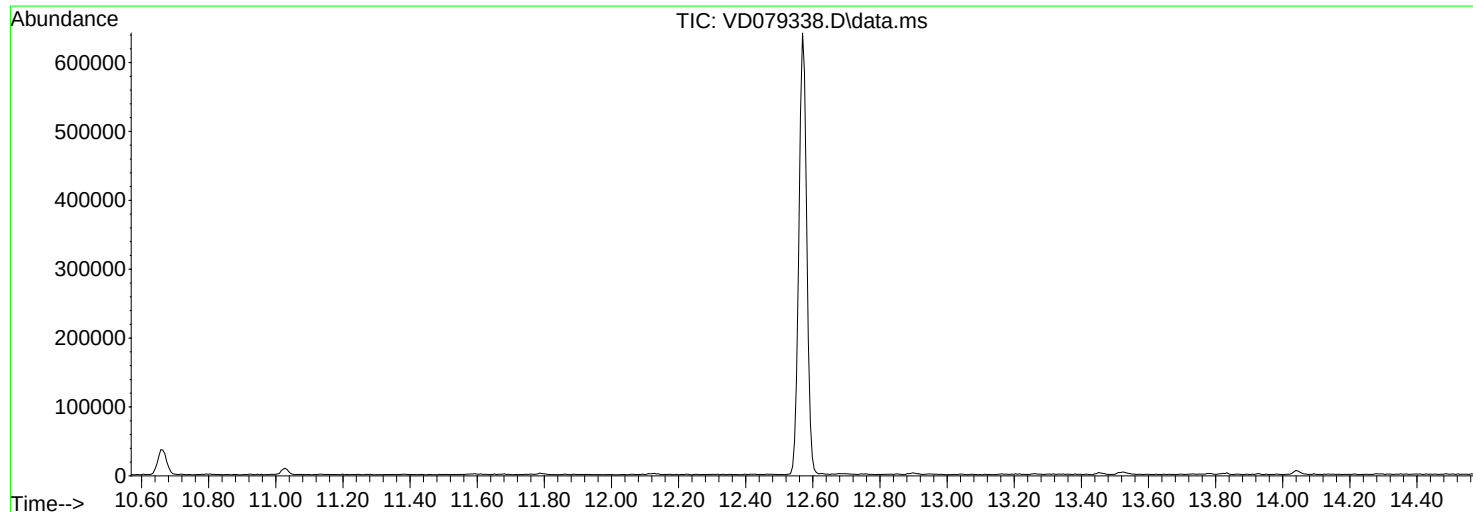

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	20877	PASS
75	95	30	60	49.9	59379	PASS
95	95	100	100	100.0	118904	PASS
96	95	5	9	6.9	8190	PASS
173	174	0.00	2	1.3	1148	PASS
174	95	50	100	76.7	91200	PASS
175	174	5	9	8.1	7408	PASS
176	174	95	101	95.8	87325	PASS
177	176	5	9	7.2	6301	PASS