
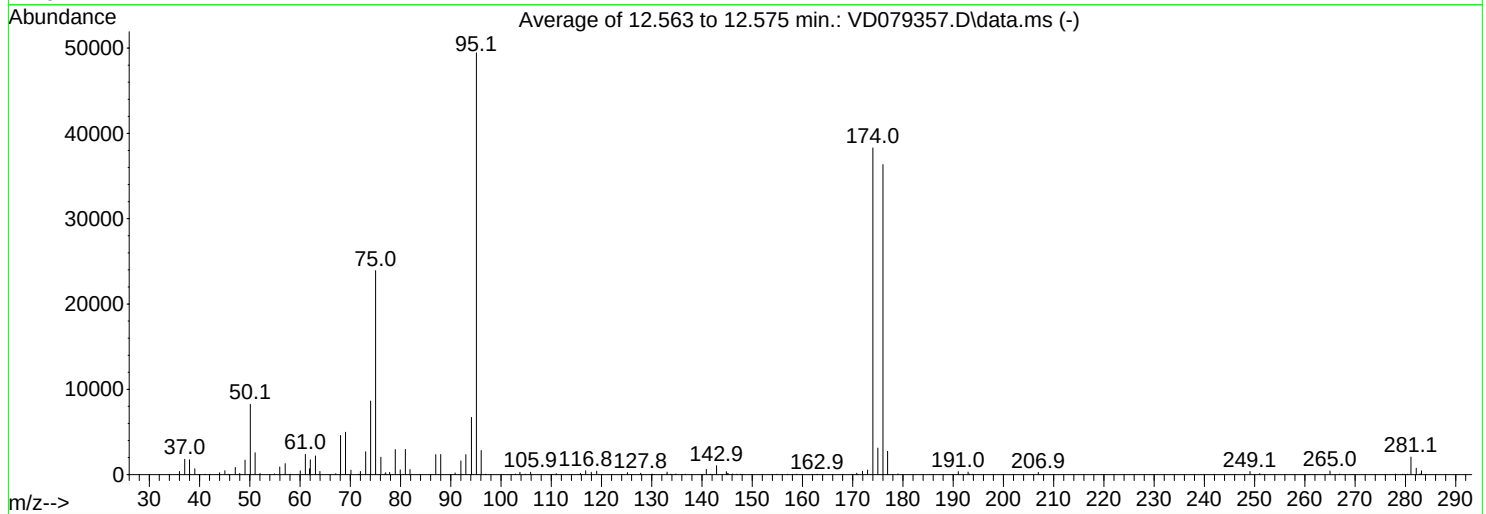


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070924\
Data File : VD079357.D
Acq On : 09 Jul 2024 11:55
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D070824S.M
Title : SW846 8260
Last Update : Mon Jul 08 17:06:59 2024

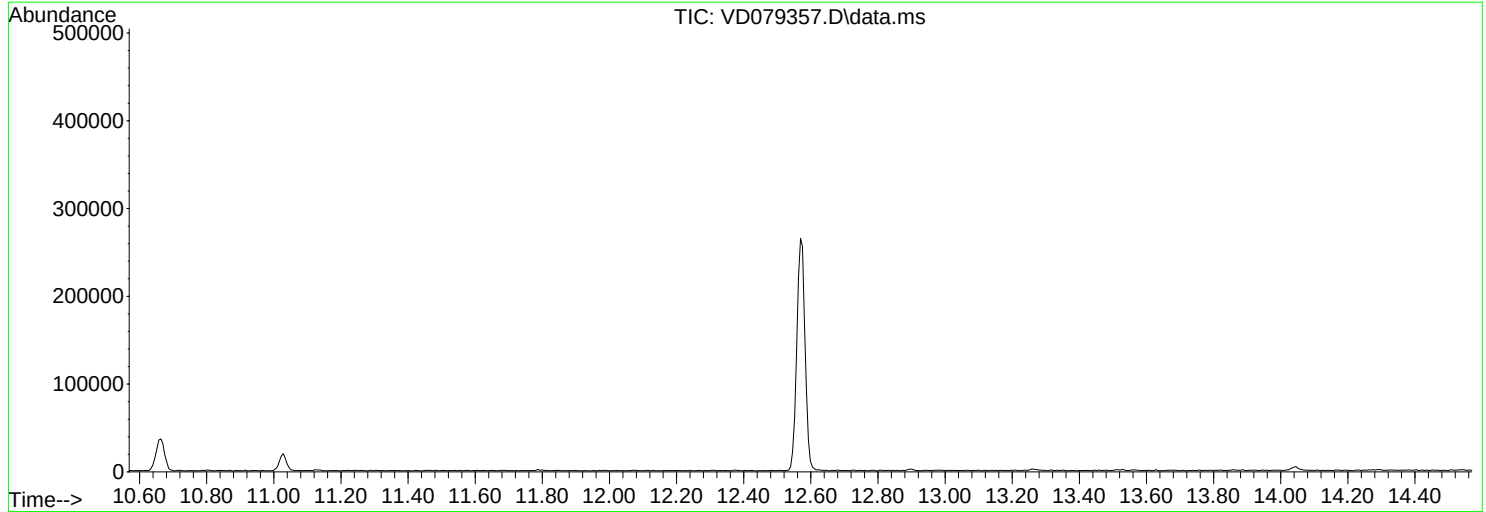

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	8254	PASS
75	95	30	60	48.3	23904	PASS
95	95	100	100	100.0	49440	PASS
96	95	5	9	5.7	2837	PASS
173	174	0.00	2	1.4	540	PASS
174	95	50	100	77.4	38288	PASS
175	174	5	9	8.1	3111	PASS
176	174	95	101	94.9	36344	PASS
177	176	5	9	7.5	2733	PASS