
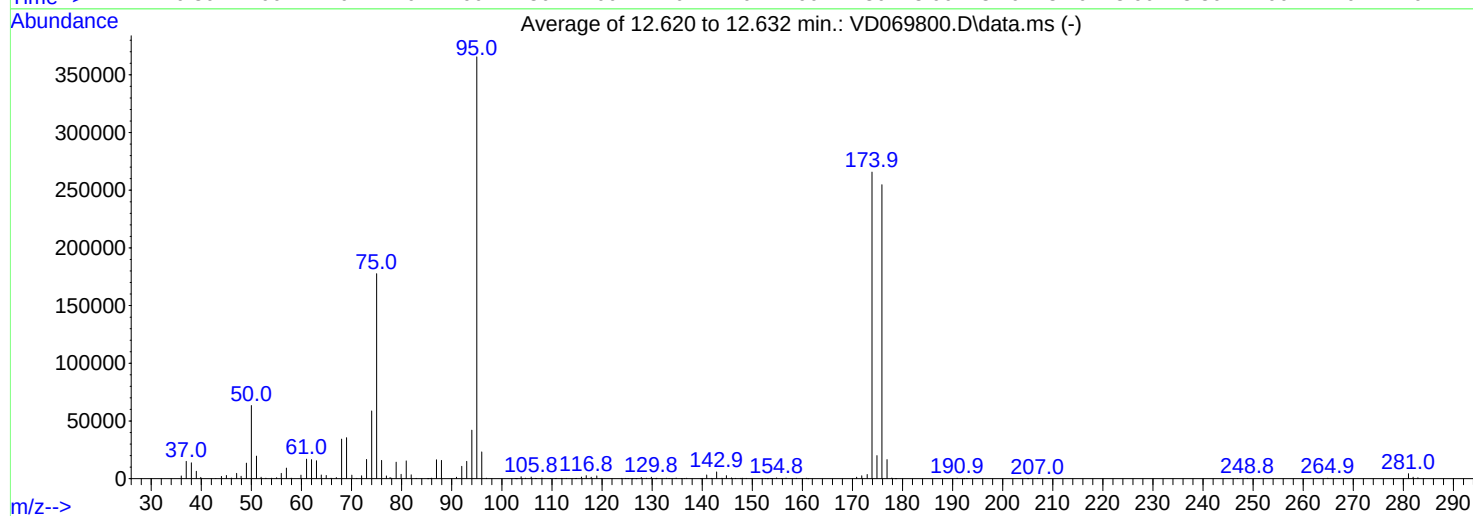


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072221\
 Data File : VD069800.D
 Acq On : 22 Jul 2021 09:14
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072221S.M
 Title : SW846 8260
 Last Update : Fri Jul 23 04:51:13 2021

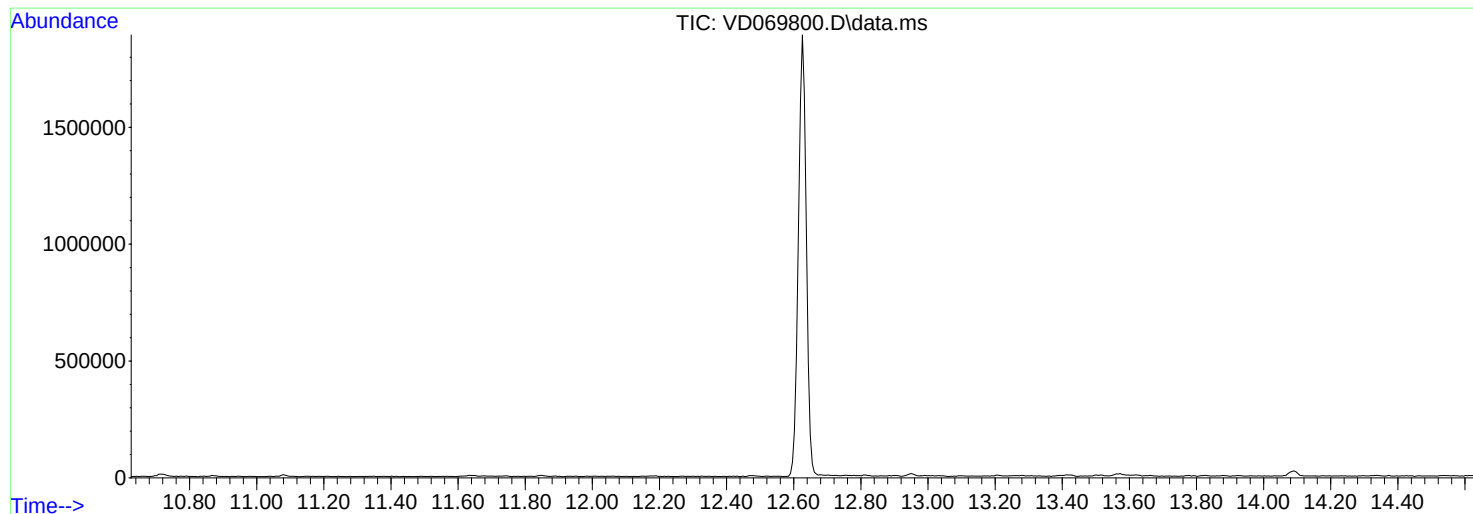

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	63397	PASS
75	95	30	60	48.6	177664	PASS
95	95	100	100	100.0	365611	PASS
96	95	5	9	6.3	23213	PASS
173	174	0.00	2	1.4	3595	PASS
174	95	50	100	72.7	265728	PASS
175	174	5	9	7.5	19931	PASS
176	174	95	101	95.9	254720	PASS
177	176	5	9	6.5	16491	PASS