
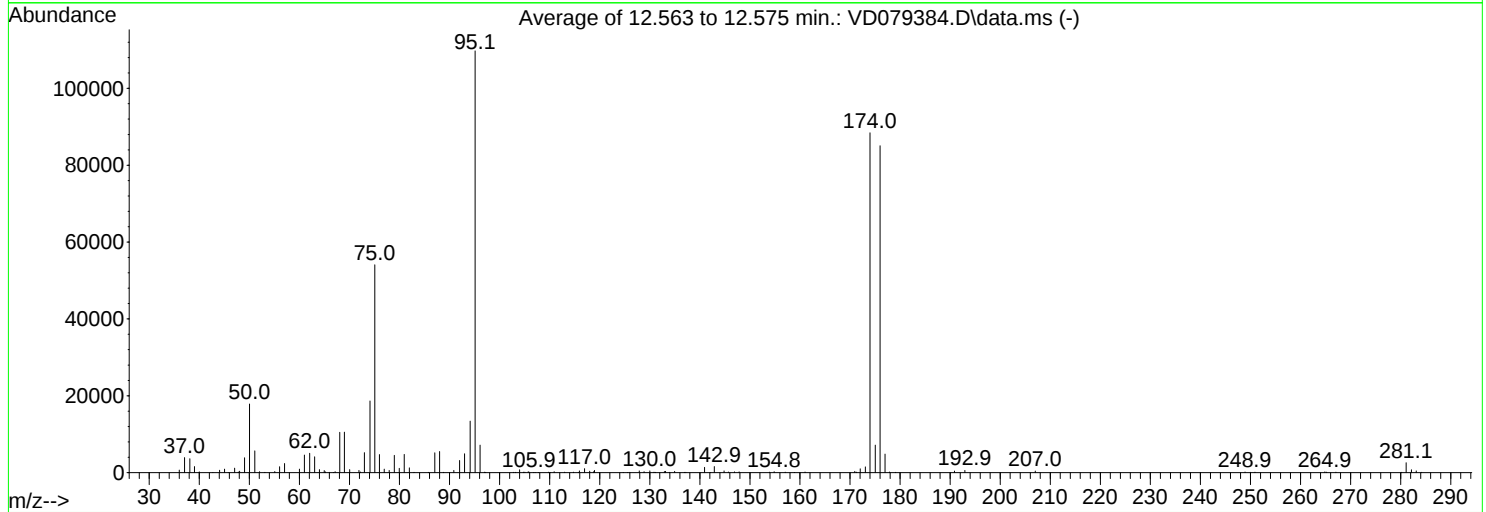


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072224\
Data File : VD079384.D
Acq On : 22 Jul 2024 09:20
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072224S.M
Title : SW846 8260
Last Update : Tue Jul 23 10:24:07 2024

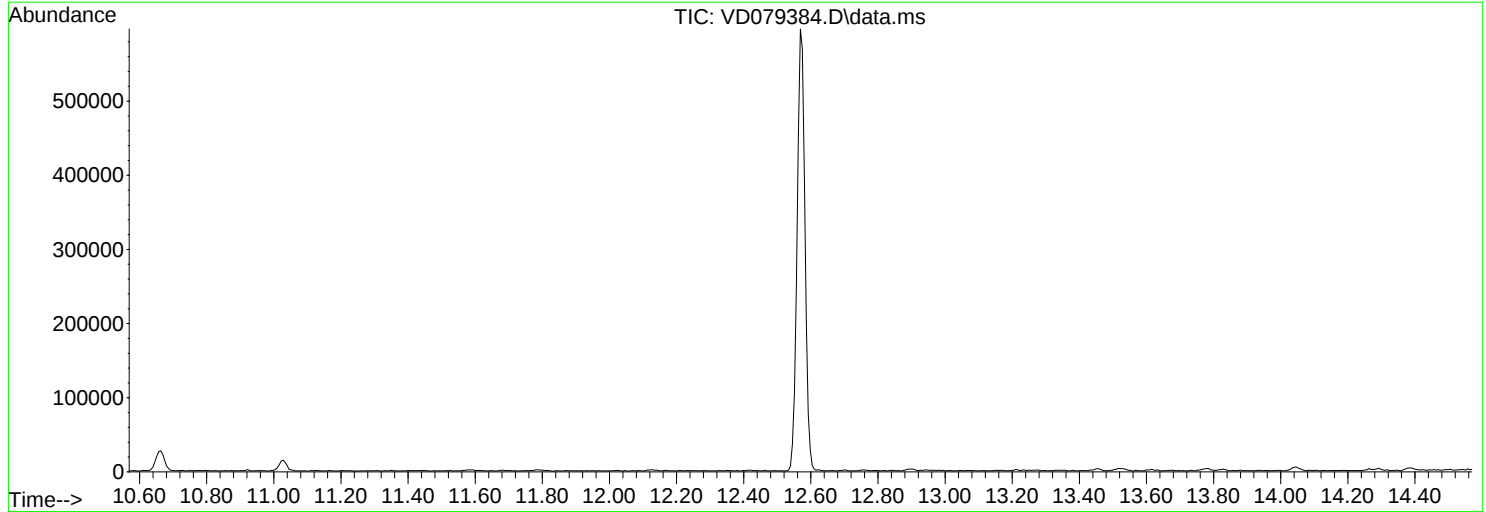

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	17851	PASS
75	95	30	60	49.3	54072	PASS
95	95	100	100	100.0	109765	PASS
96	95	5	9	6.5	7179	PASS
173	174	0.00	2	1.7	1509	PASS
174	95	50	100	80.6	88429	PASS
175	174	5	9	8.1	7159	PASS
176	174	95	101	96.2	85056	PASS
177	176	5	9	5.7	4855	PASS