
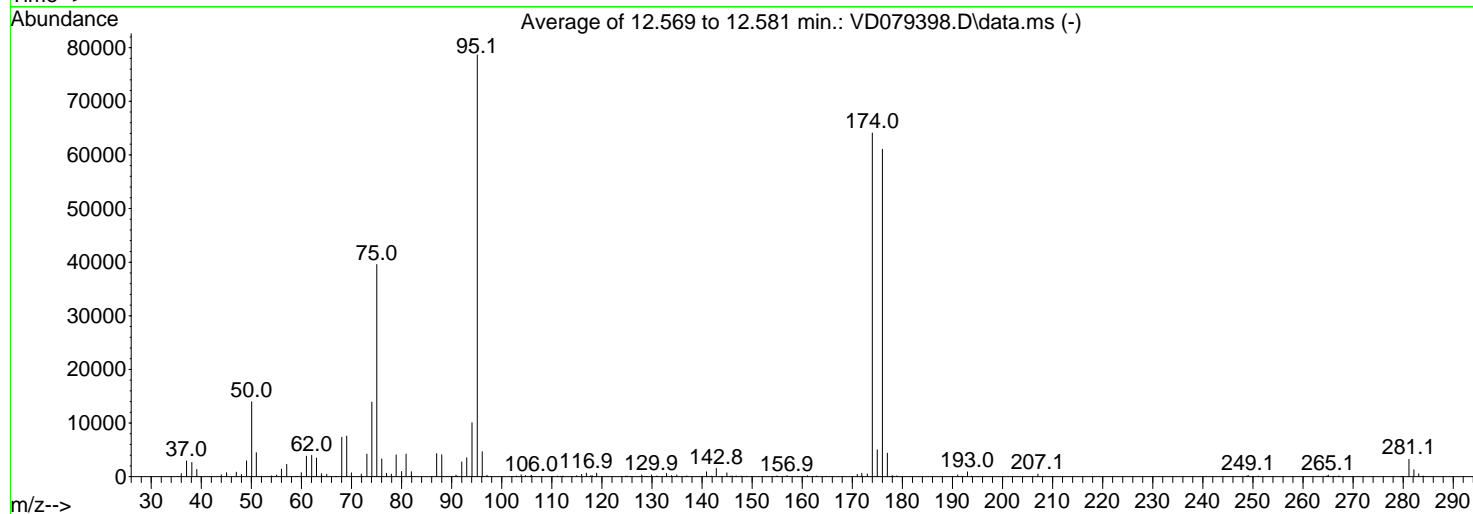


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072524\
 Data File : VD079398.D
 Acq On : 25 Jul 2024 08:51
 Operator : RP/MD
 Sample : BFB
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072524S.M
 Title : SW846 8260
 Last Update : Fri Jul 26 12:23:49 2024

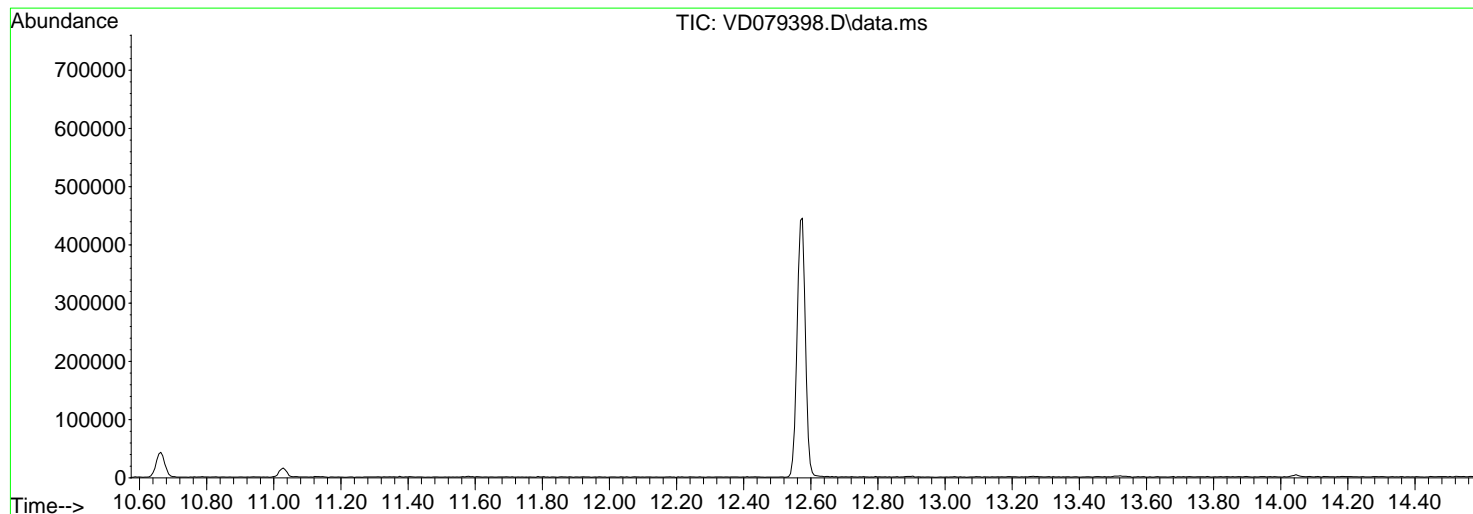

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	13956	PASS
75	95	30	60	50.3	39579	PASS
95	95	100	100	100.0	78664	PASS
96	95	5	9	5.9	4649	PASS
173	174	0.00	2	0.8	497	PASS
174	95	50	100	81.5	64099	PASS
175	174	5	9	7.8	5001	PASS
176	174	95	101	95.3	61056	PASS
177	176	5	9	7.2	4386	PASS