
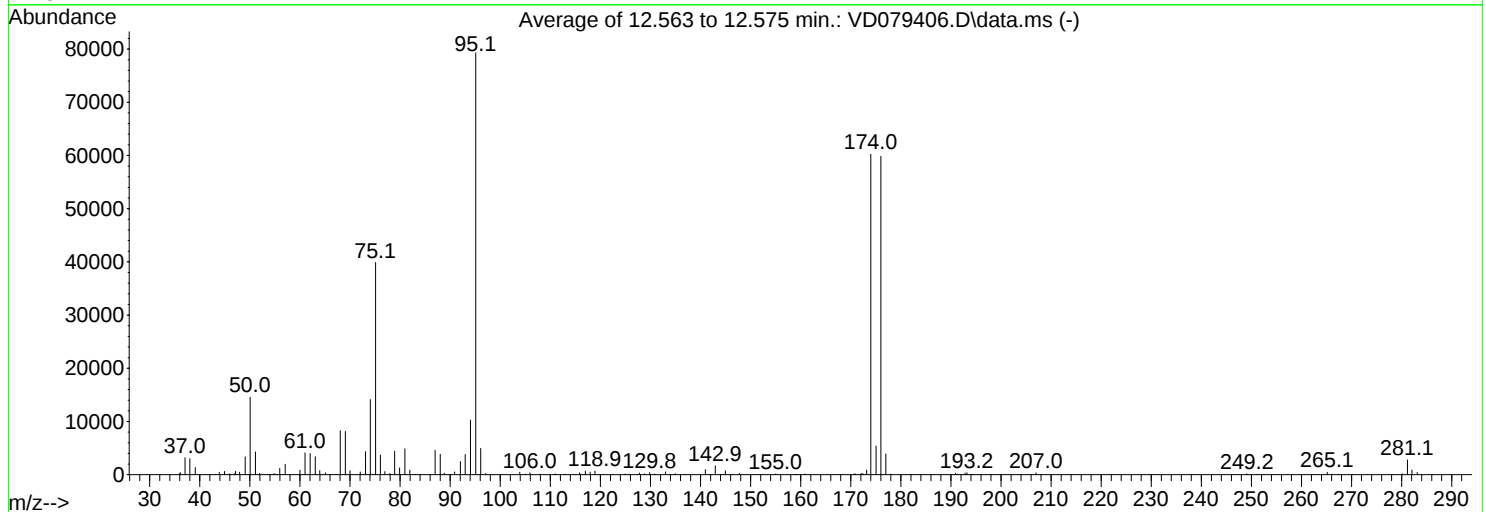


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD072624\
Data File : VD079406.D
Acq On : 26 Jul 2024 11:11
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072524S.M
Title : SW846 8260
Last Update : Fri Jul 26 12:23:49 2024

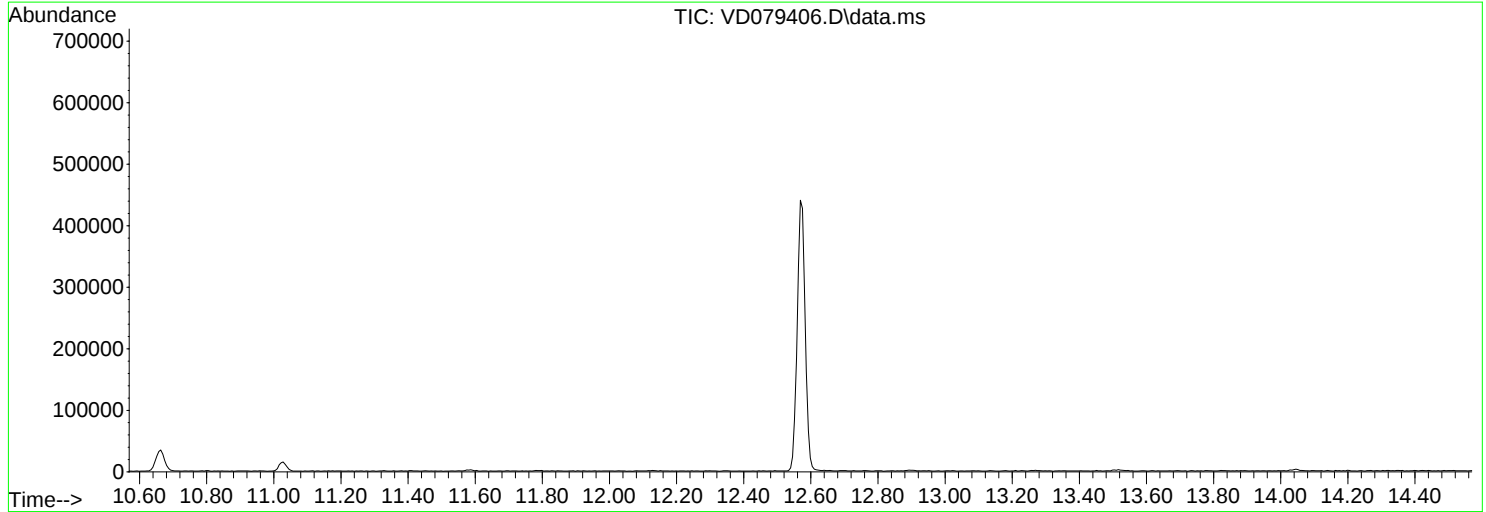

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	14559	PASS
75	95	30	60	50.3	39885	PASS
95	95	100	100	100.0	79291	PASS
96	95	5	9	6.2	4922	PASS
173	174	0.00	2	1.5	886	PASS
174	95	50	100	75.9	60221	PASS
175	174	5	9	8.9	5377	PASS
176	174	95	101	99.4	59869	PASS
177	176	5	9	6.5	3893	PASS