
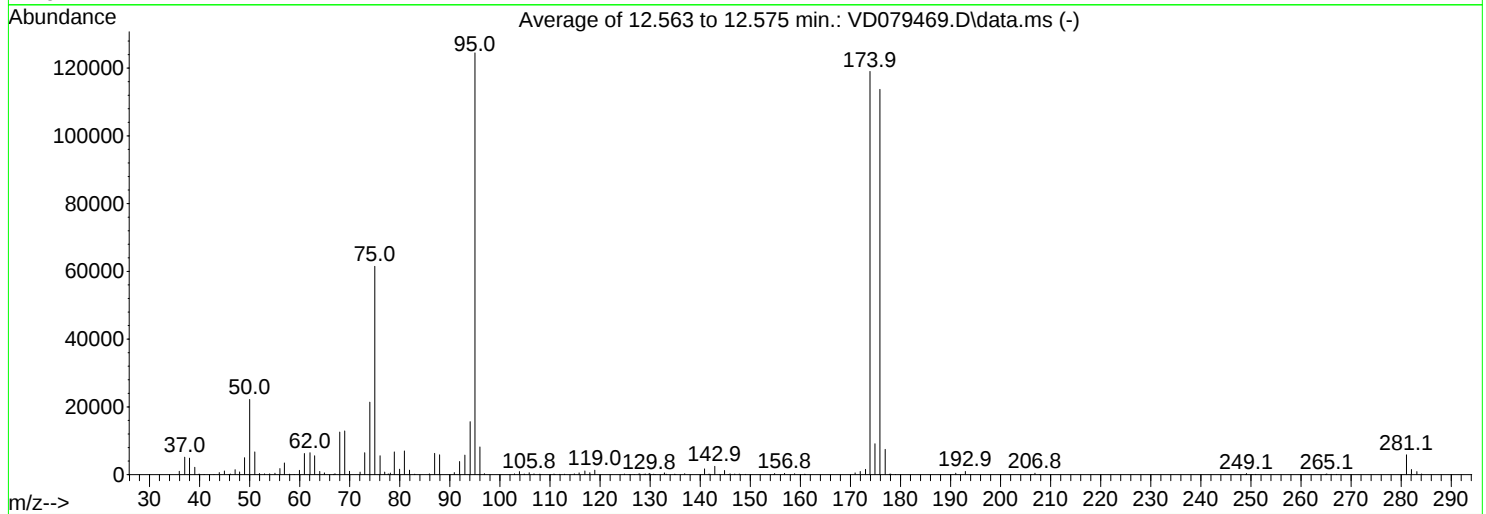


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD073024\
Data File : VD079469.D
Acq On : 30 Jul 2024 20:55
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

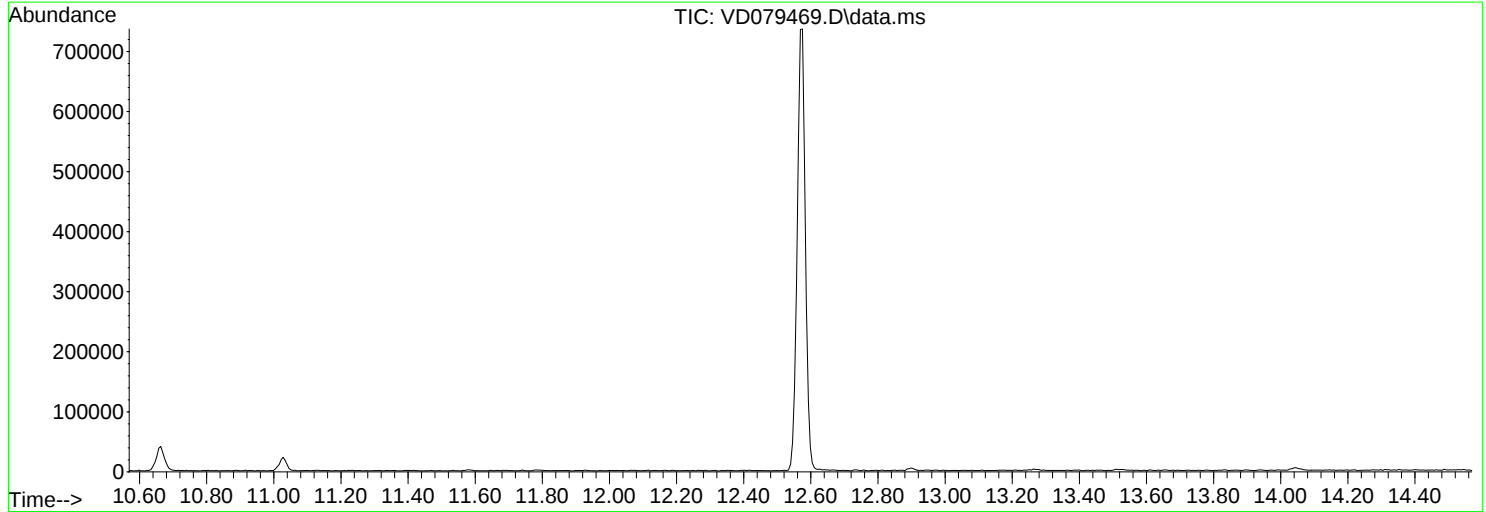

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	22221	PASS
75	95	30	60	49.4	61496	PASS
95	95	100	100	100.0	124509	PASS
96	95	5	9	6.6	8186	PASS
173	174	0.00	2	1.3	1578	PASS
174	95	50	100	95.6	119005	PASS
175	174	5	9	7.7	9104	PASS
176	174	95	101	95.6	113739	PASS
177	176	5	9	6.6	7469	PASS