
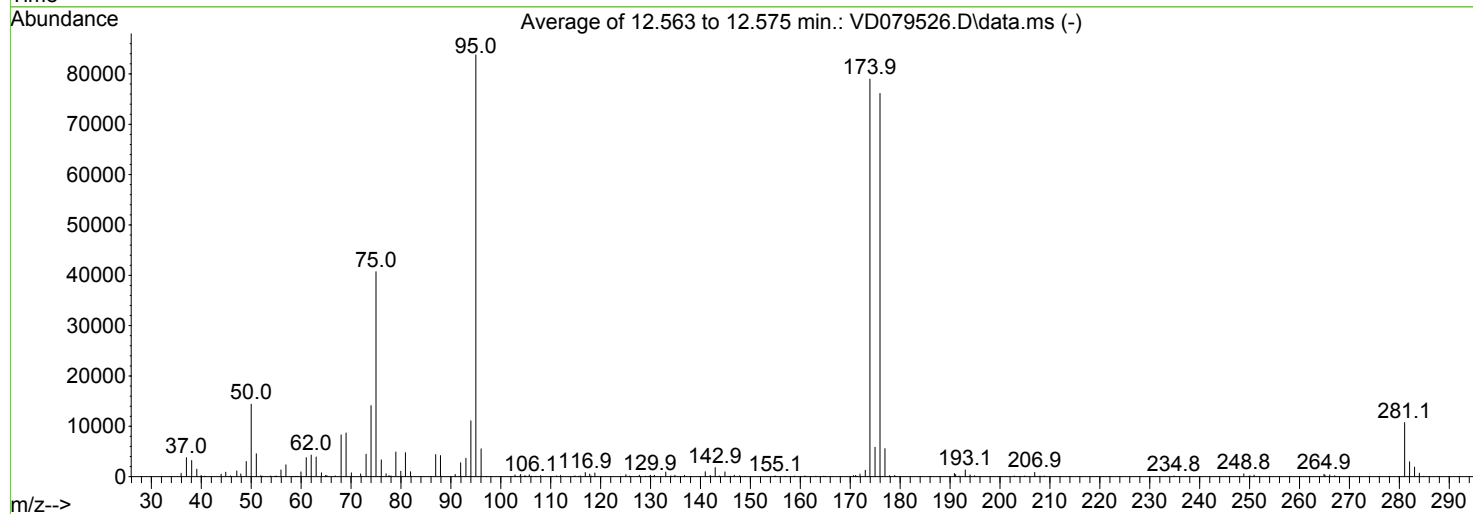


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080124\
Data File : VD079526.D
Acq On : 01 Aug 2024 09:37
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

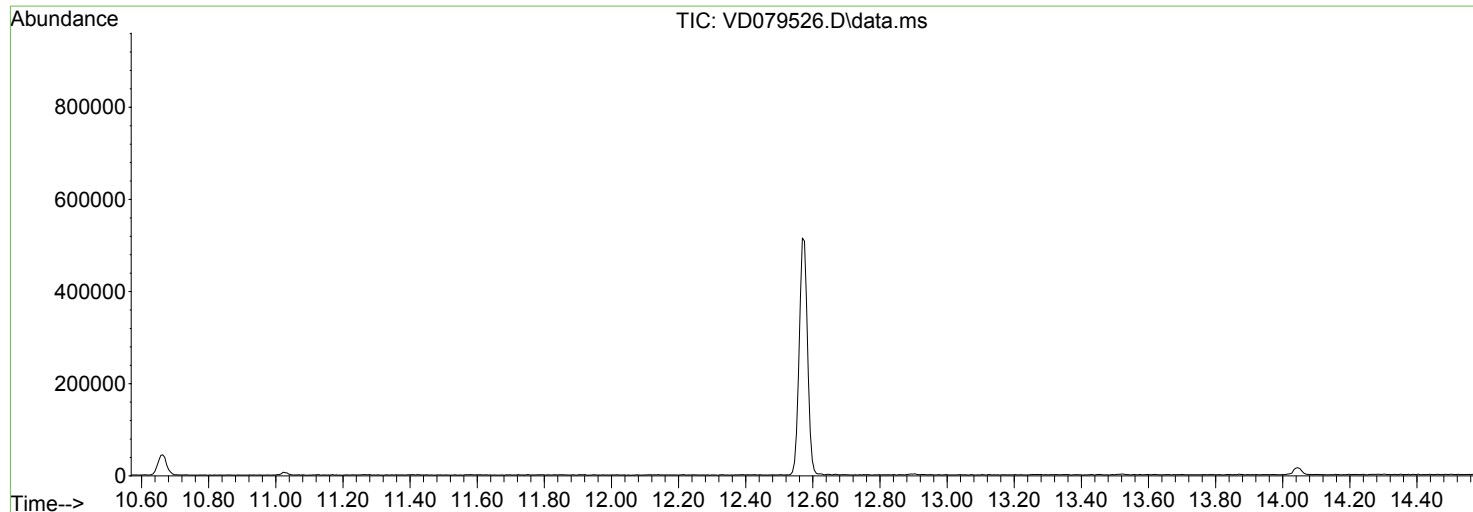

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	14389	PASS
75	95	30	60	48.6	40717	PASS
95	95	100	100	100.0	83795	PASS
96	95	5	9	6.6	5530	PASS
173	174	0.00	2	1.6	1284	PASS
174	95	50	100	94.3	78989	PASS
175	174	5	9	7.4	5840	PASS
176	174	95	101	96.4	76141	PASS
177	176	5	9	7.3	5562	PASS