

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080524\
 Data File : VD079608.D
 Acq On : 06 Aug 2024 05:34
 Operator : RP/MD
 Sample : P3464-01
 Misc : 4.54G/5.0ml/MSVOA_D/SOIL/A
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Aug 06 08:09:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 30 03:50:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	86401	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	148639	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	91044	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	22742	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	47376	53.974	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	107.940%
35) Dibromofluoromethane	7.805	113	53290	52.969	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.940%
50) Toluene-d8	10.269	98	119791	30.661	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	61.320%
62) 4-Bromofluorobenzene	12.569	95	20875	18.464	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	36.920%


Target Compounds					Qvalue	
5) Bromomethane	2.699	94	139	Below Cal	#	40
13) Acrolein	3.922	56	62	Below Cal	#	15
16) Acetone	4.022	43	241	1.413	ug/l #	37
20) Methylene Chloride	4.799	84	18345	Below Cal		98
27) cis-1,2-Dichloroethene	7.081	96	1296	1.081	ug/l	74
31) Cyclohexane	7.875	56	2007	1.377	ug/l #	23
36) 1,1-Dichloropropene	7.875	75	6764	4.926	ug/l #	45
38) Carbon Tetrachloride	7.875	117	8007	5.547	ug/l #	18
76) 1,2,3-Trichloropropane	12.569	75	10705	53.851	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.569	75	10705	102.709	ug/l #	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080524\
Data File : VD079608.D
Acq On : 06 Aug 2024 05:34
Operator : RP/MD
Sample : P3464-01
Misc : 4.54G/5.0ml/MSVOA_D/SOIL/A
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :


Quant Time: Aug 06 08:09:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Quant Title : SW846 8260
QLast Update : Tue Jul 30 03:50:47 2024
Response via : Initial Calibration

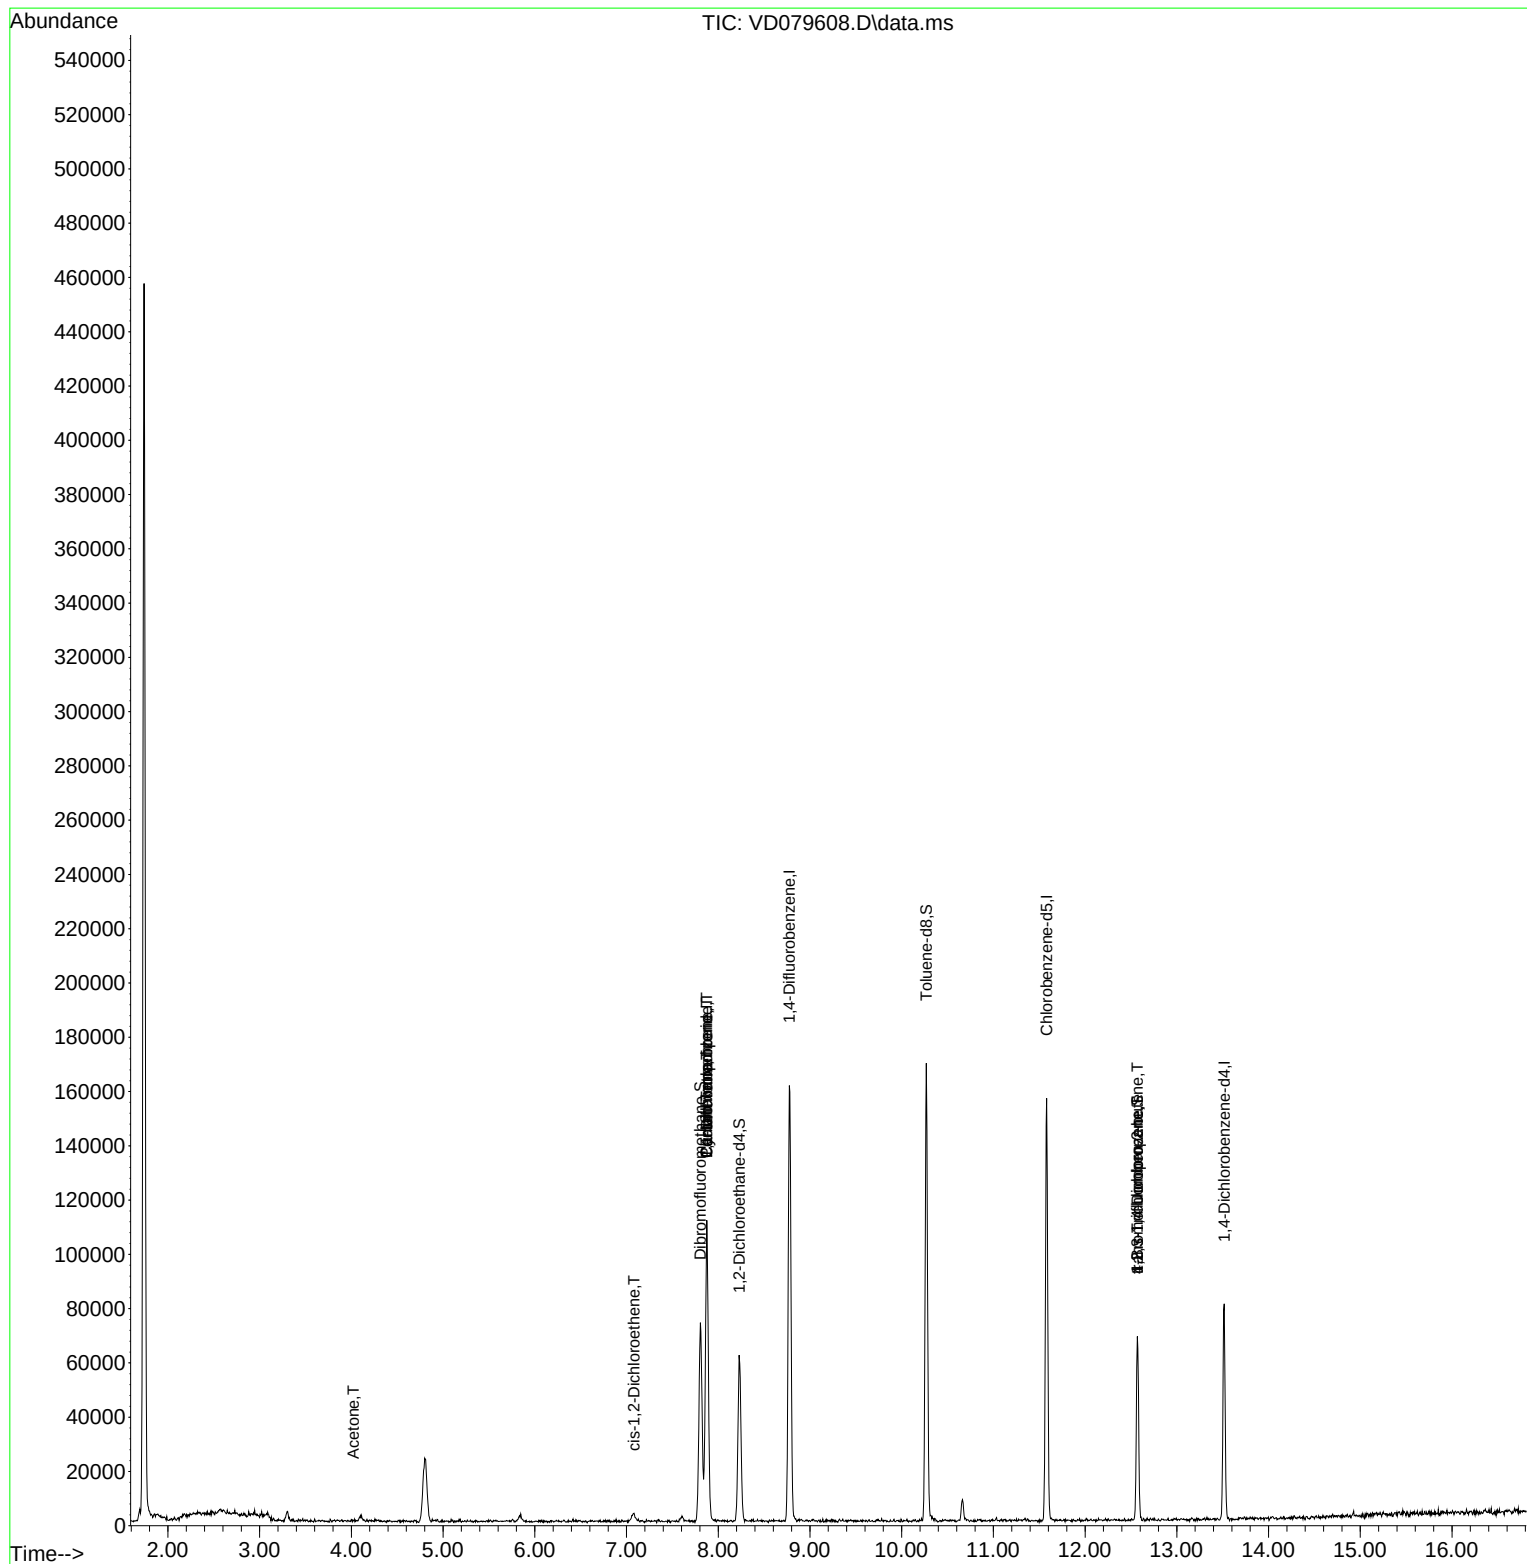



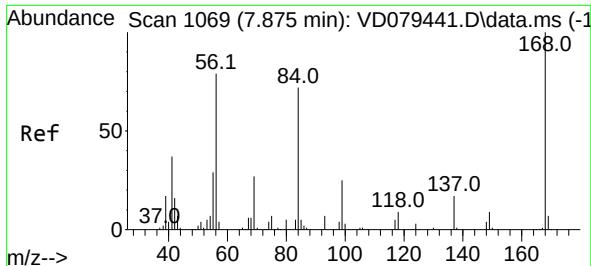


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Instrument :
MSVOA_D
ClientSampleId :



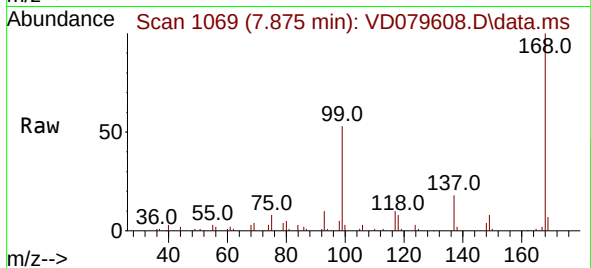



Tgt Ion:168 Resp: 86401
Ion Ratio Lower Upper
168 100
99 53.3 41.1 61.7

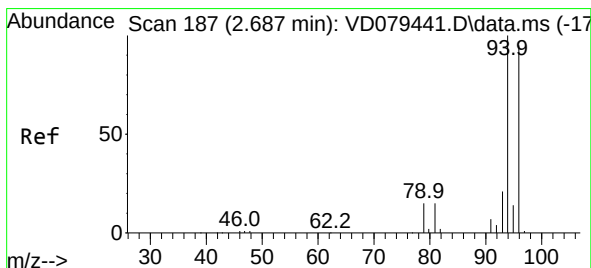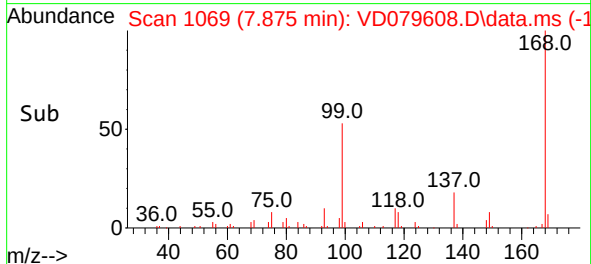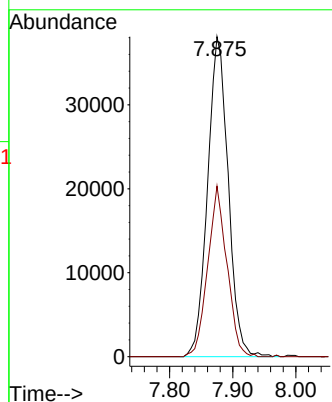

#5
Bromomethane
Concen: Below Cal
RT: 2.699 min Scan# 189
Delta R.T. 0.012 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Tgt Ion: 94 Resp: 139
Ion Ratio Lower Upper
94 100
96 154.7 76.9 115.3#


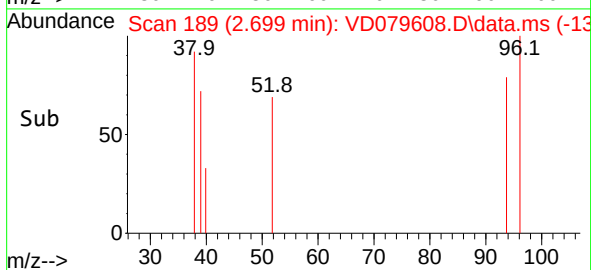
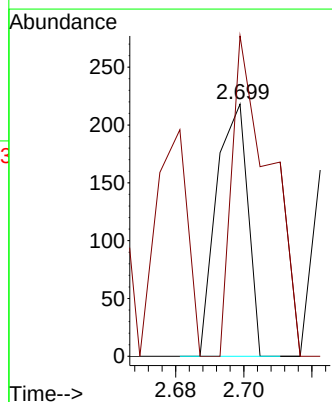
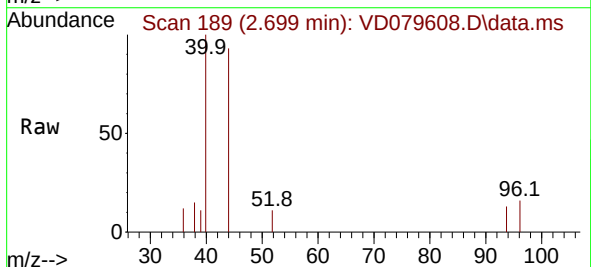


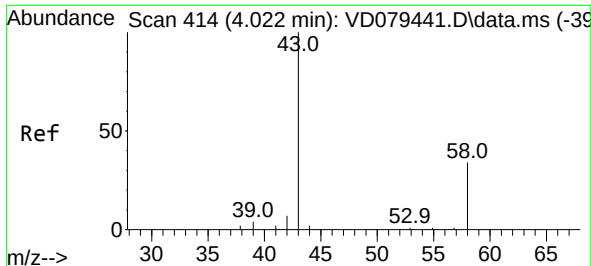

#16
Acetone
Concen: 1.413 ug/l
RT: 4.022 min Scan# 414
Delta R.T. -0.000 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 241
Ion Ratio Lower Upper
43 100
58 0.0 30.4 45.6#

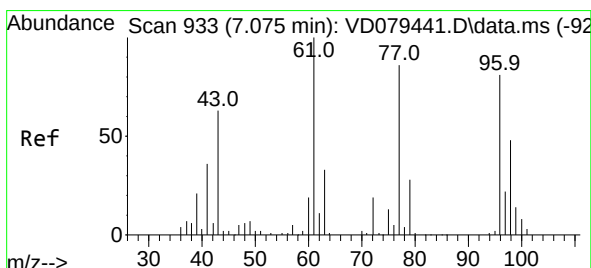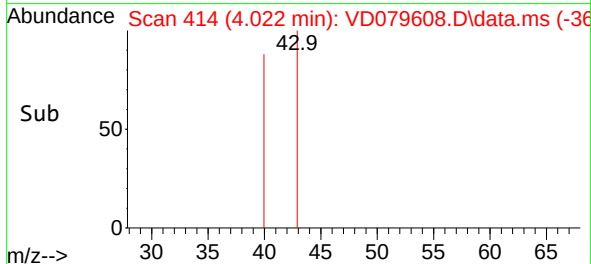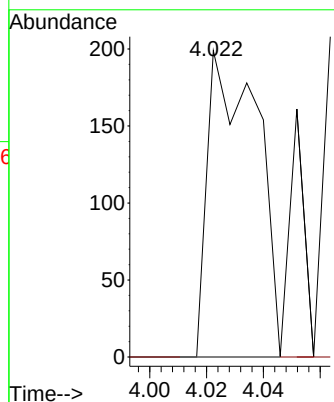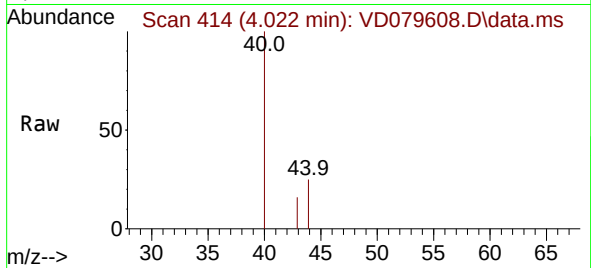

#27
cis-1,2-Dichloroethene
Concen: 1.081 ug/l
RT: 7.081 min Scan# 934
Delta R.T. 0.006 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34


Tgt Ion: 96 Resp: 1296
Ion Ratio Lower Upper
96 100
61 85.6 0.0 229.0
98 44.4 0.0 127.2

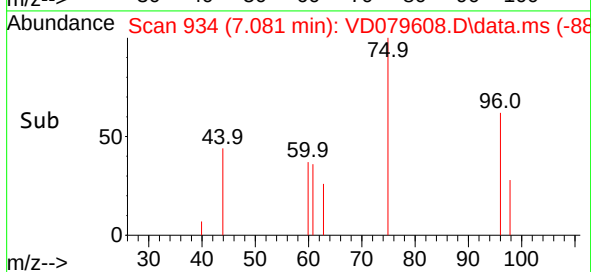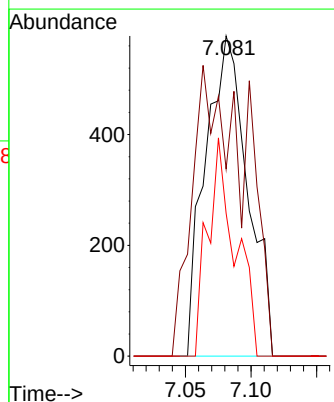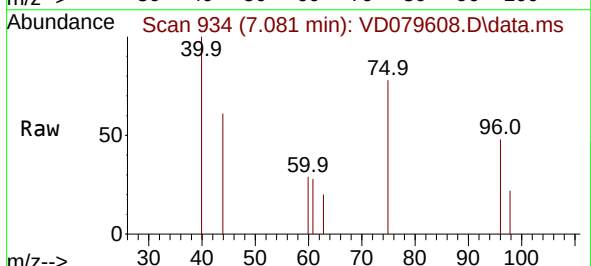



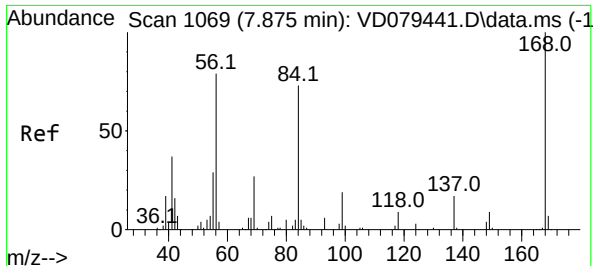


#31
Cyclohexane
Concen: 1.377 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.006 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Instrument :
MSVOA_D
ClientSampleId :



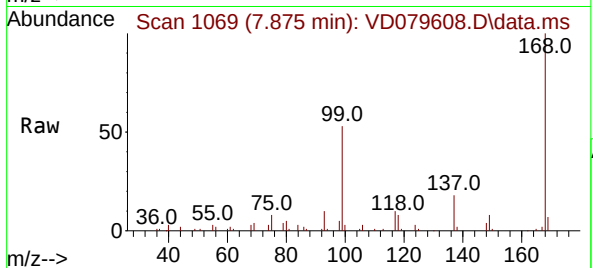



Tgt Ion: 56 Resp: 2007
Ion Ratio Lower Upper
56 100
69 167.0 28.0 42.0#
84 139.0 87.4 131.0#

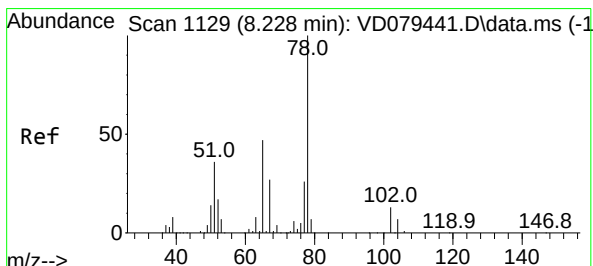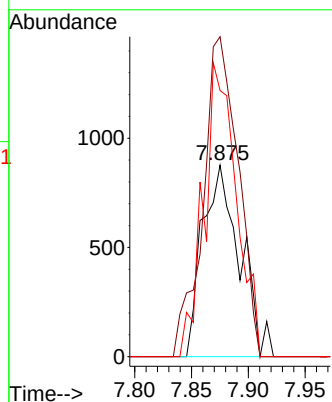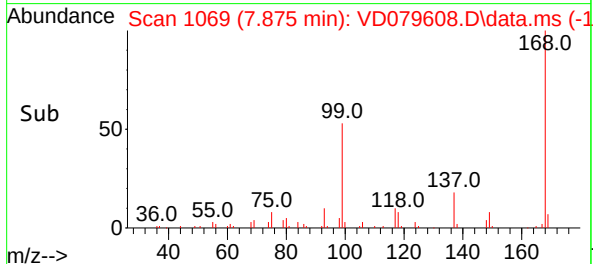

#33
1,2-Dichloroethane-d4
Concen: 53.974 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Tgt Ion: 65 Resp: 47376
Ion Ratio Lower Upper
65 100
67 56.1 0.0 111.0

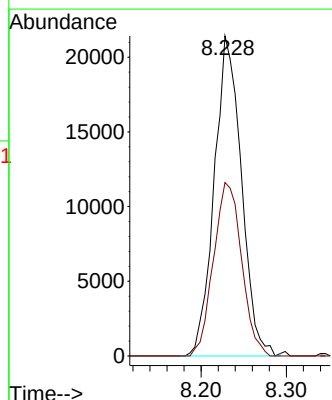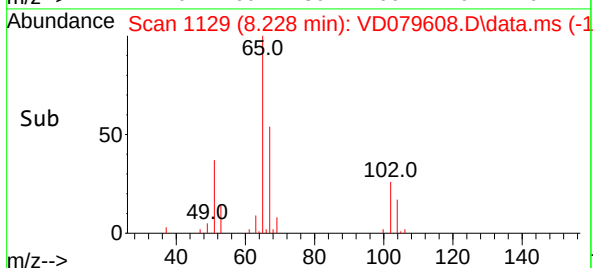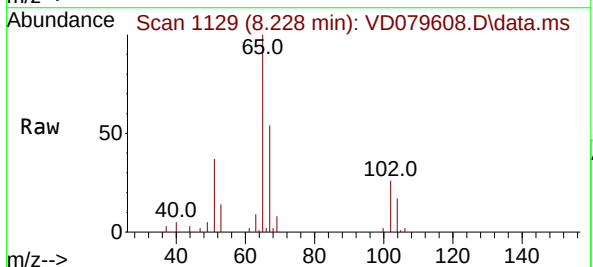

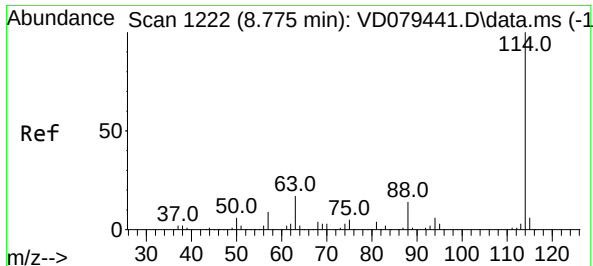

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD079608.D

Acq: 06 Aug 2024 05:34

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:114 Resp: 148639

Ion Ratio Lower Upper

114 100

63 17.6 0.0 34.0

88 14.7 0.0 27.2

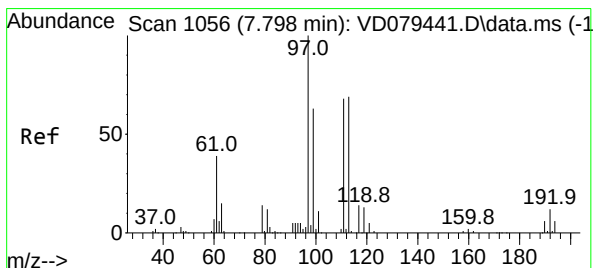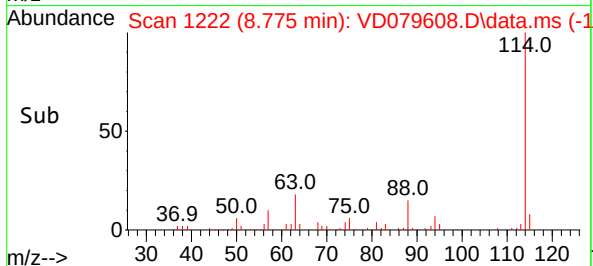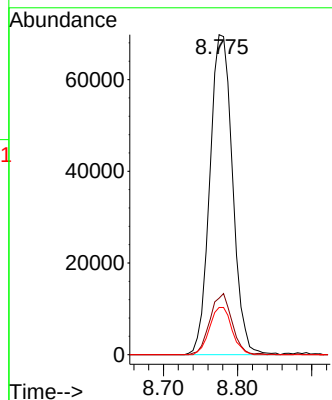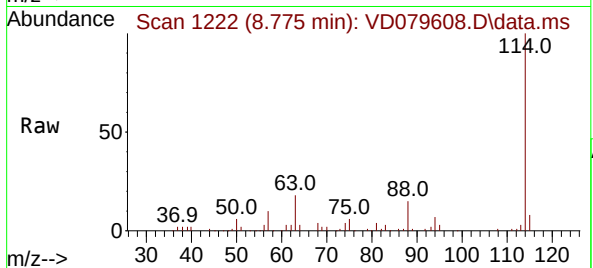

#35

Dibromofluoromethane

Concen: 52.969 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD079608.D

Acq: 06 Aug 2024 05:34




Tgt Ion:113 Resp: 53290


Ion Ratio Lower Upper

113 100

111 102.7 84.0 126.0

192 19.1 15.4 23.0

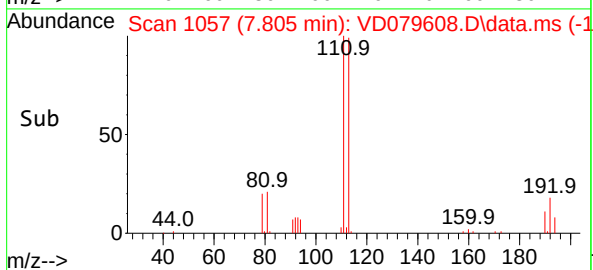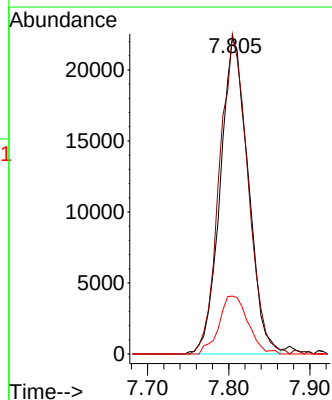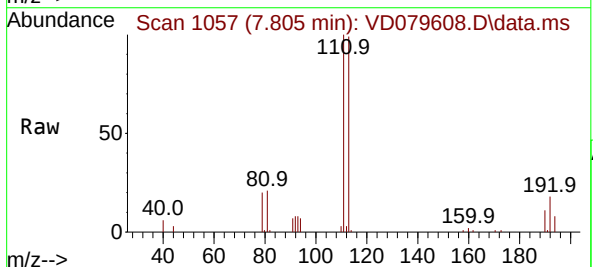

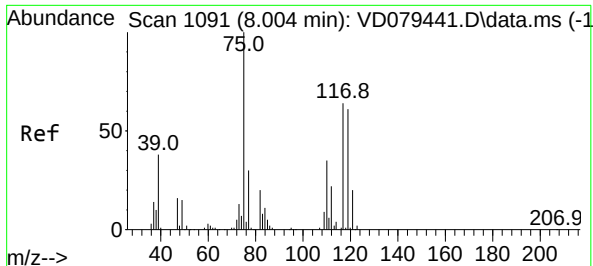

#36

1,1-Dichloropropene

Concen: 4.926 ug/l

RT: 7.875 min Scan# 1069

Delta R.T. -0.135 min

Lab File: VD079608.D





Acq: 06 Aug 2024 05:34

Instrument :

MSVOA_D

ClientSampleId :

Tgt Ion:	75	Resp:	6764
Ion	Ratio	Lower	Upper
75	100		
110	6.5	19.6	58.7#
77	0.0	26.1	39.1#

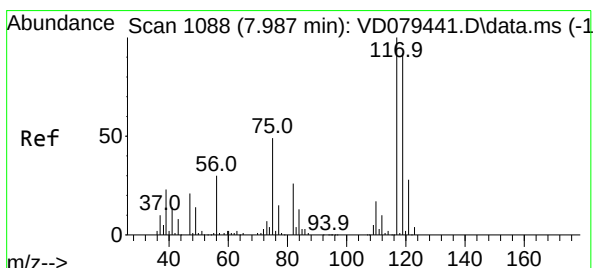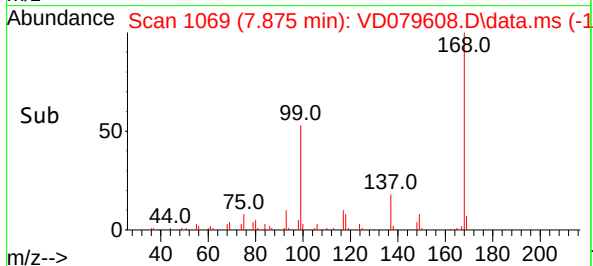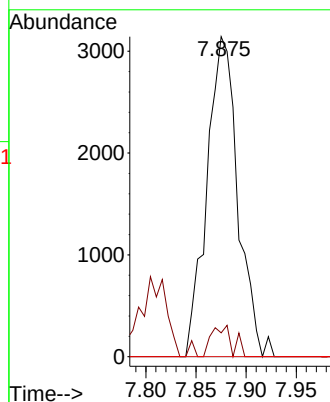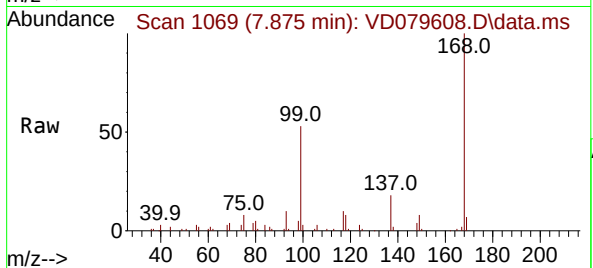

#38

Carbon Tetrachloride

Concen: 5.547 ug/l




RT: 7.875 min Scan# 1069


Delta R.T. -0.112 min

Lab File: VD079608.D

Acq: 06 Aug 2024 05:34

Tgt Ion:	117	Resp:	8007
Ion	Ratio	Lower	Upper
117	100		
119	6.3	75.4	113.0#
121	0.0	25.0	37.4#


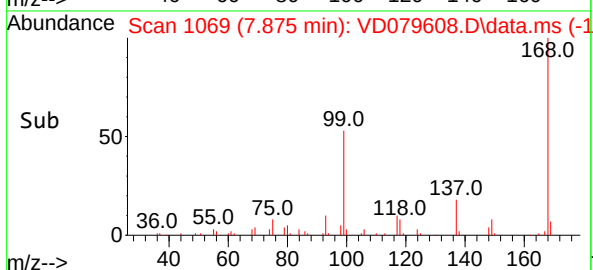
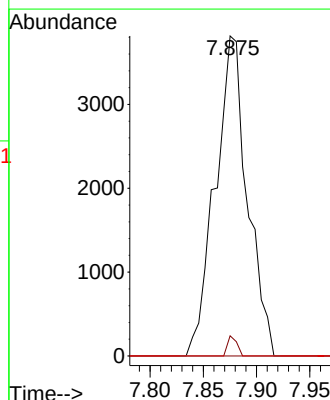
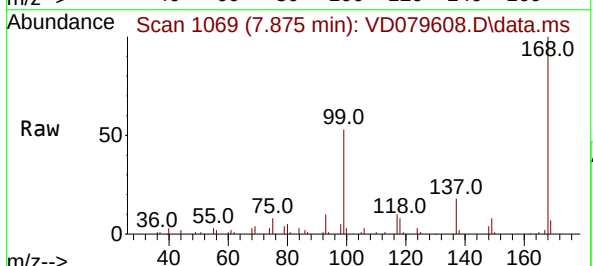


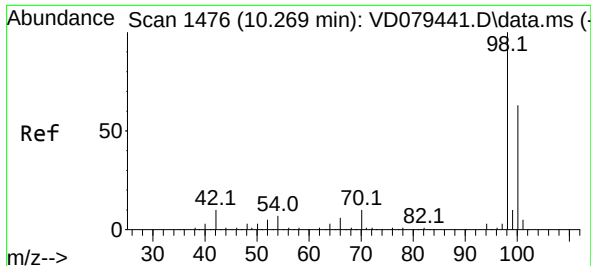

#50
Toluene-d8
Concen: 30.661 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 98 Resp: 119791
Ion Ratio Lower Upper
98 100
100 63.8 51.6 77.4

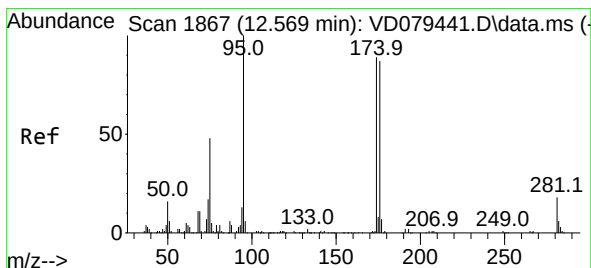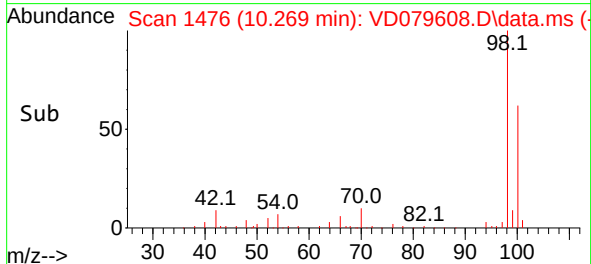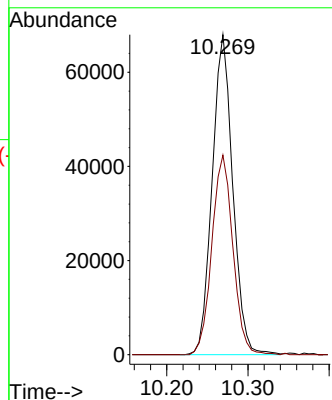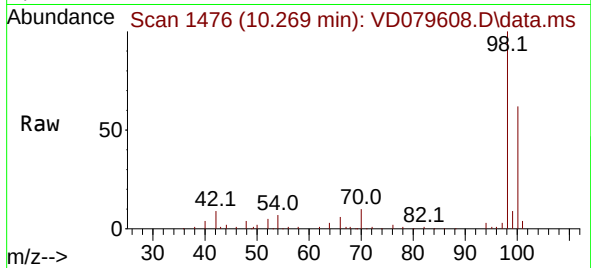

#62
4-Bromofluorobenzene
Concen: 18.464 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.000 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Tgt Ion: 95 Resp: 20875
Ion Ratio Lower Upper
95 100
174 100.6 0.0 195.4
176 95.6 0.0 192.6


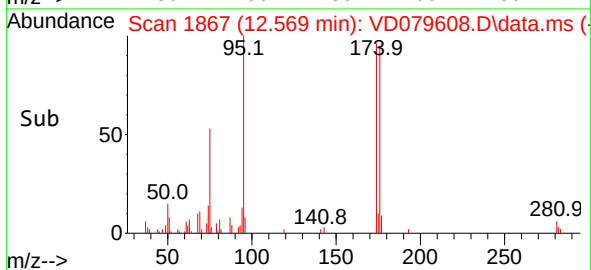
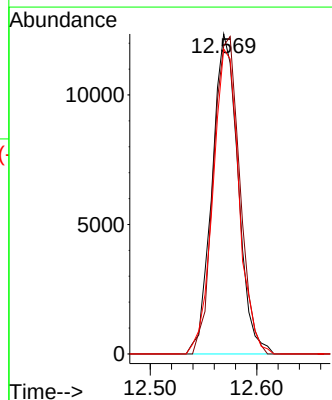
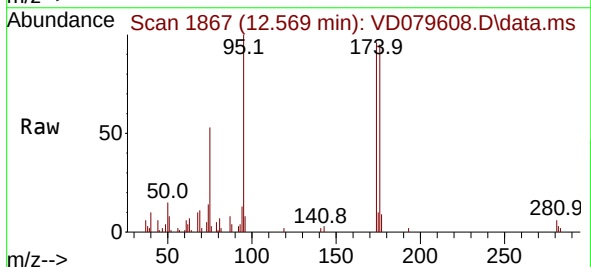


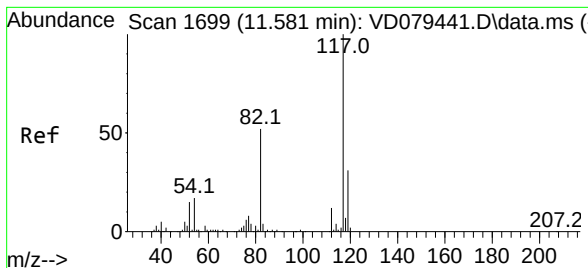

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
117	100		
82	50.4	39.8	59.6
119	32.2	25.7	38.5

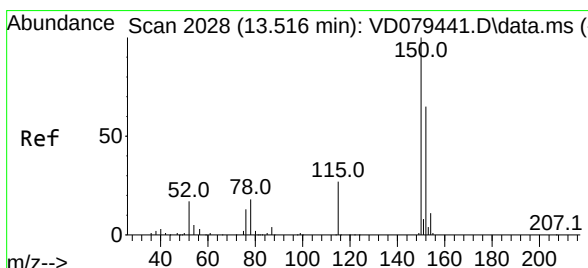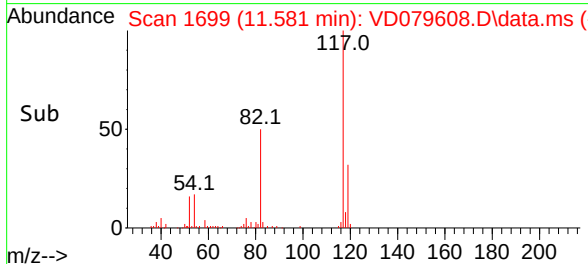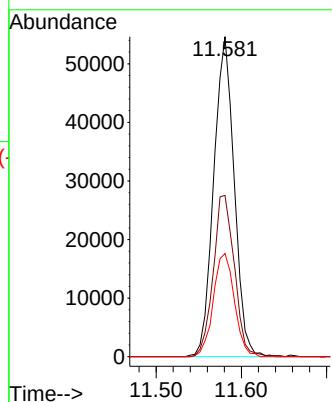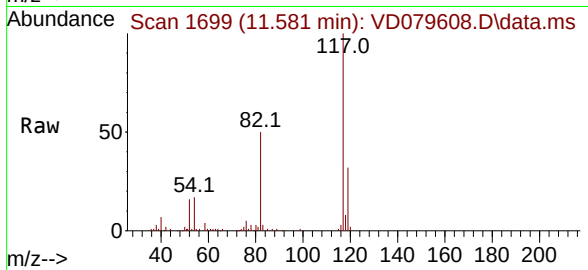

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.006 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Tgt Ion	Ratio	Lower	Upper
152	100		
115	50.3	26.5	79.5
150	161.4	0.0	341.6


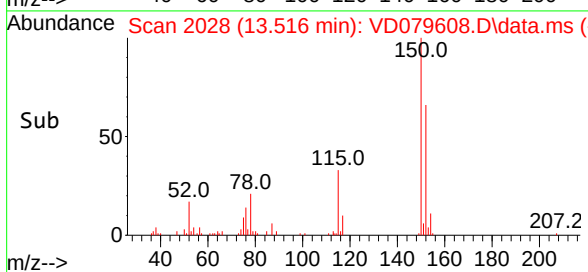
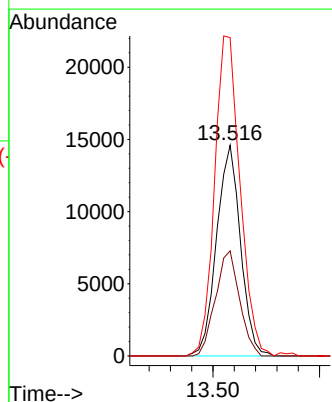
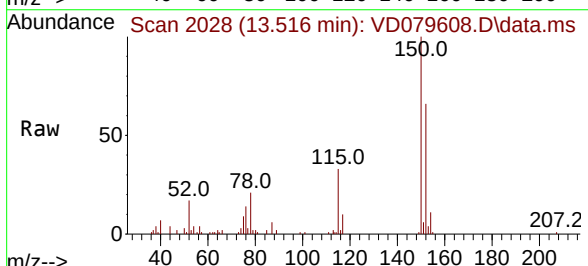


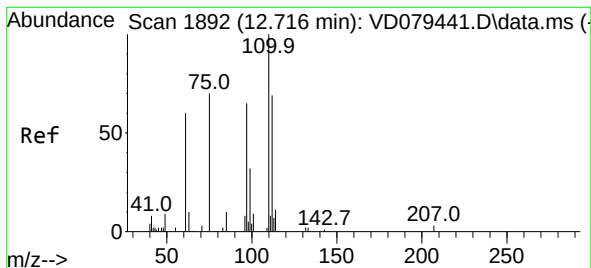

#76
1,2,3-Trichloropropane
Concen: 53.851 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. -0.153 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Instrument :
MSVOA_D
ClientSampleId :

Tgt Ion: 75 Resp: 10705
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

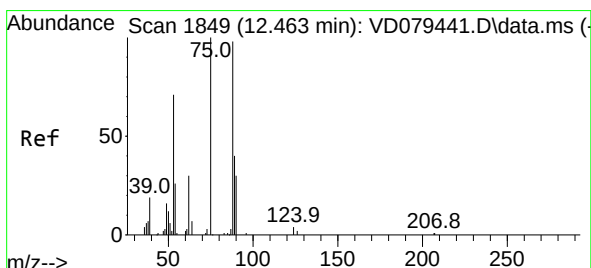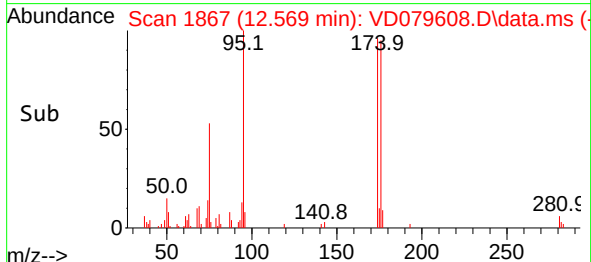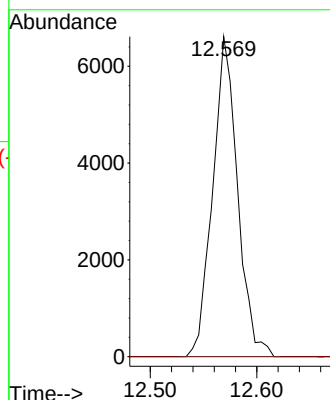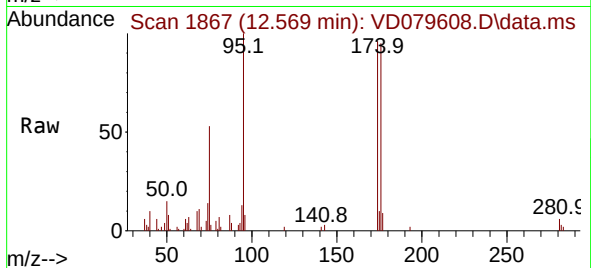

#81
trans-1,4-Dichloro-2-butene
Concen: 102.709 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. 0.100 min
Lab File: VD079608.D
Acq: 06 Aug 2024 05:34

Tgt Ion: 75 Resp: 10705
Ion Ratio Lower Upper
75 100
53 0.0 61.4 92.2#
89 0.0 35.4 53.0#

