
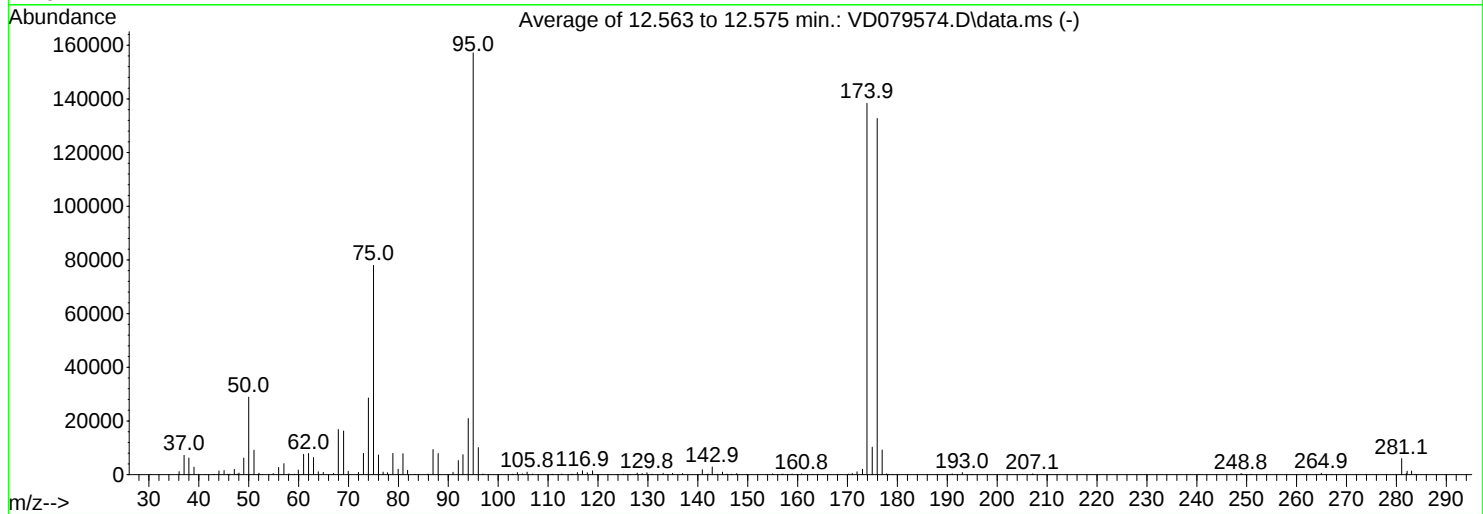


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080524\
Data File : VD079574.D
Acq On : 05 Aug 2024 09:41
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

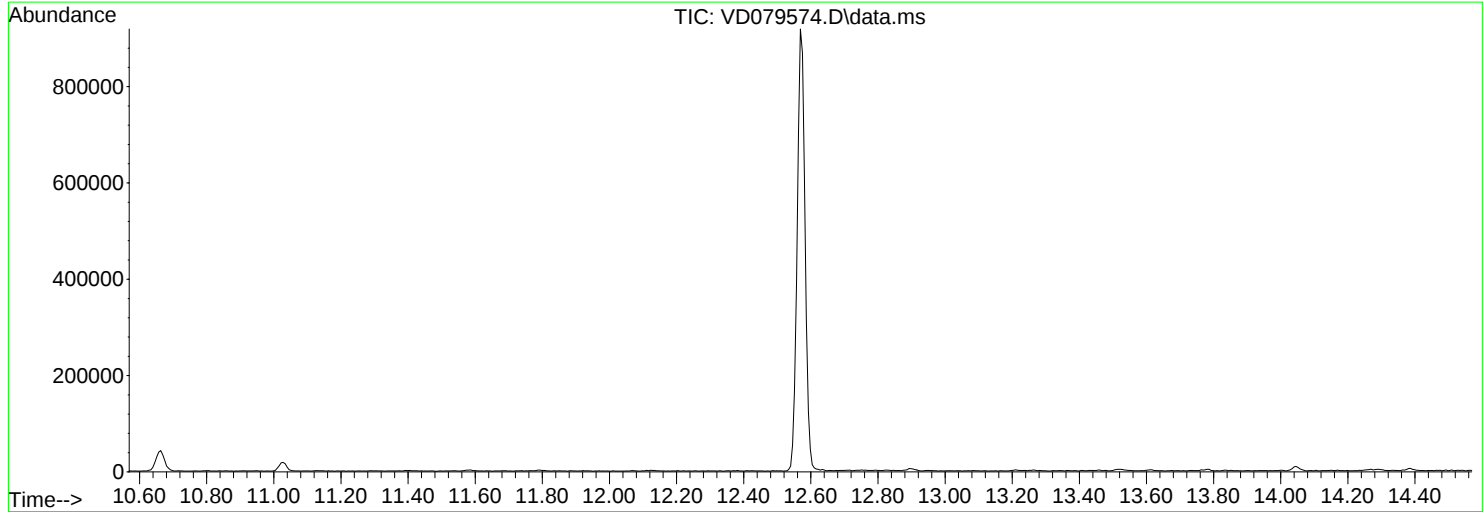

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	28859	PASS
75	95	30	60	49.6	77989	PASS
95	95	100	100	100.0	157163	PASS
96	95	5	9	6.4	10095	PASS
173	174	0.00	2	1.5	2014	PASS
174	95	50	100	88.1	138397	PASS
175	174	5	9	7.4	10235	PASS
176	174	95	101	95.9	132680	PASS
177	176	5	9	6.9	9160	PASS