
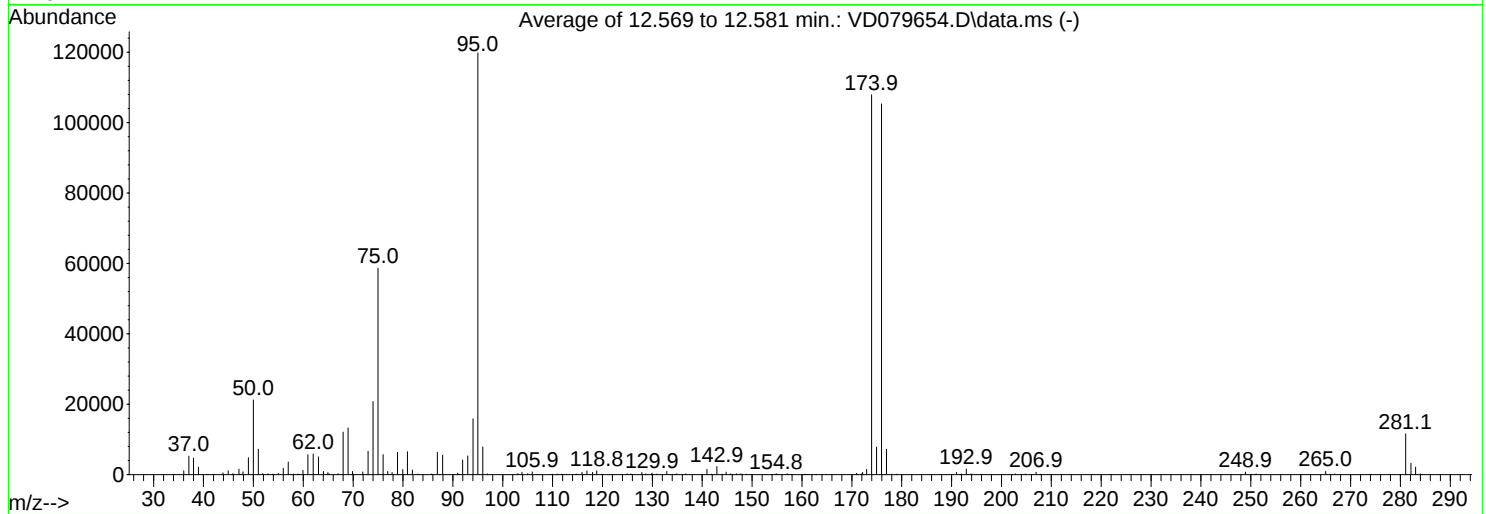


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080724\
Data File : VD079654.D
Acq On : 07 Aug 2024 21:41
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

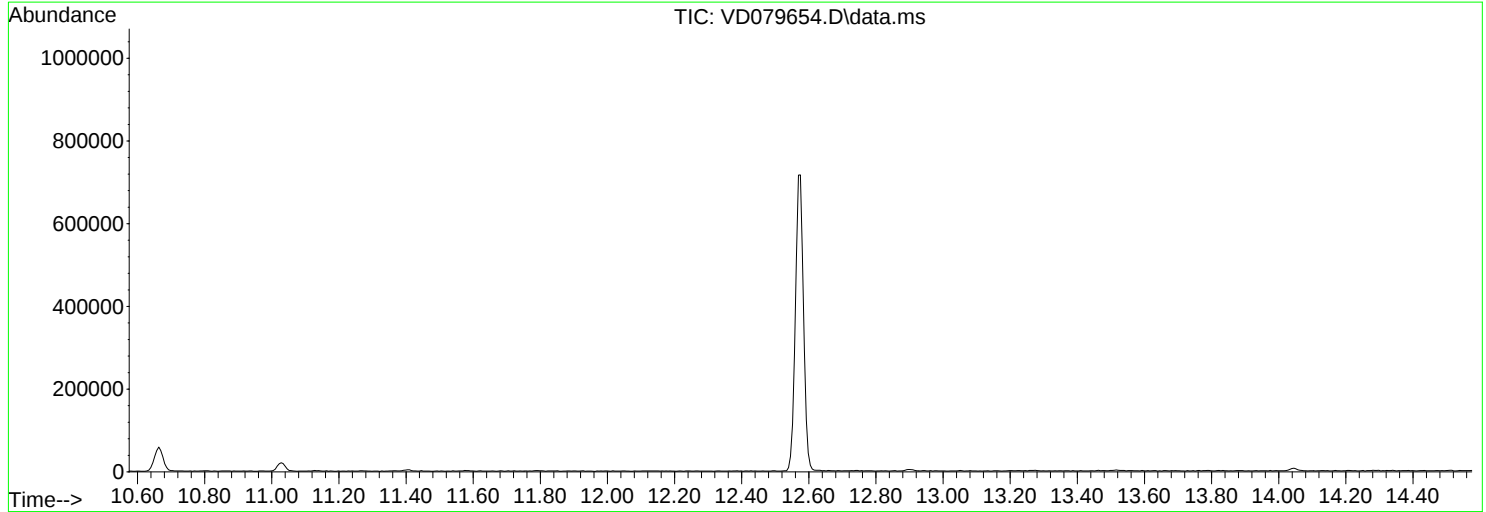

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	21248	PASS
75	95	30	60	48.9	58627	PASS
95	95	100	100	100.0	119835	PASS
96	95	5	9	6.6	7891	PASS
173	174	0.00	2	1.4	1491	PASS
174	95	50	100	90.1	107928	PASS
175	174	5	9	7.3	7838	PASS
176	174	95	101	97.6	105331	PASS
177	176	5	9	6.8	7209	PASS