
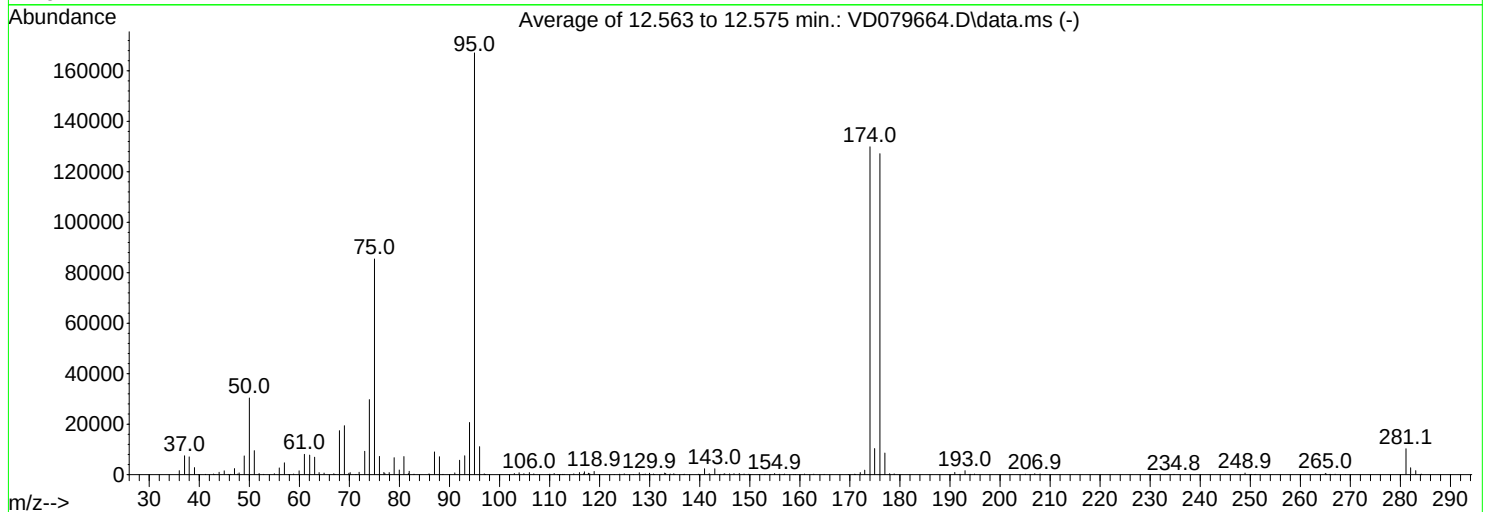


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080824\
Data File : VD079664.D
Acq On : 08 Aug 2024 13:10
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D072924S.M
Title : SW846 8260
Last Update : Tue Jul 30 03:50:47 2024

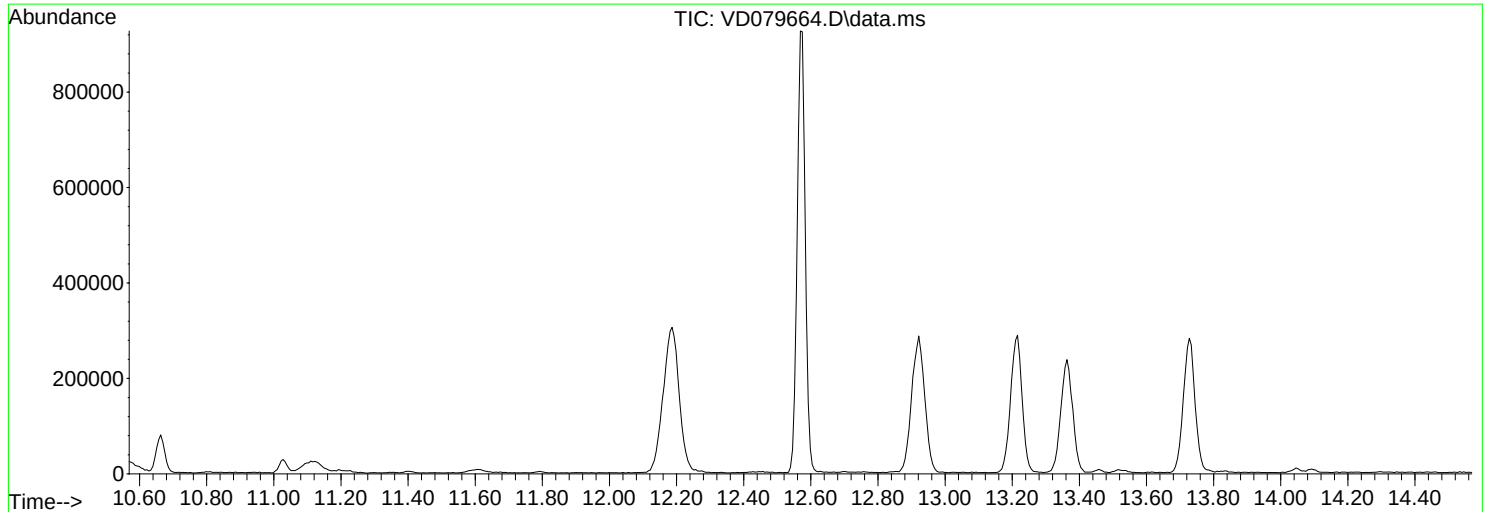

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	30379	PASS
75	95	30	60	51.1	85445	PASS
95	95	100	100	100.0	167125	PASS
96	95	5	9	6.6	11081	PASS
173	174	0.00	2	1.4	1771	PASS
174	95	50	100	77.7	129931	PASS
175	174	5	9	8.0	10342	PASS
176	174	95	101	97.9	127195	PASS
177	176	5	9	6.8	8594	PASS