
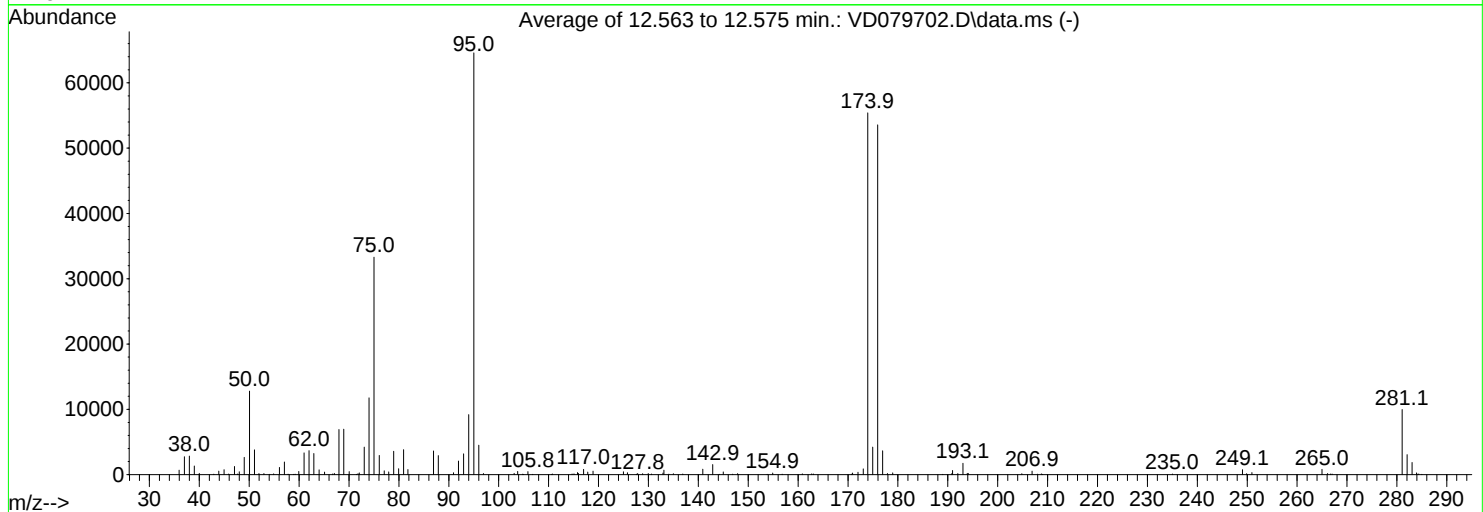


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD081224\
Data File : VD079702.D
Acq On : 12 Aug 2024 09:54
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081224S.M
Title : SW846 8260
Last Update : Tue Aug 13 01:06:11 2024

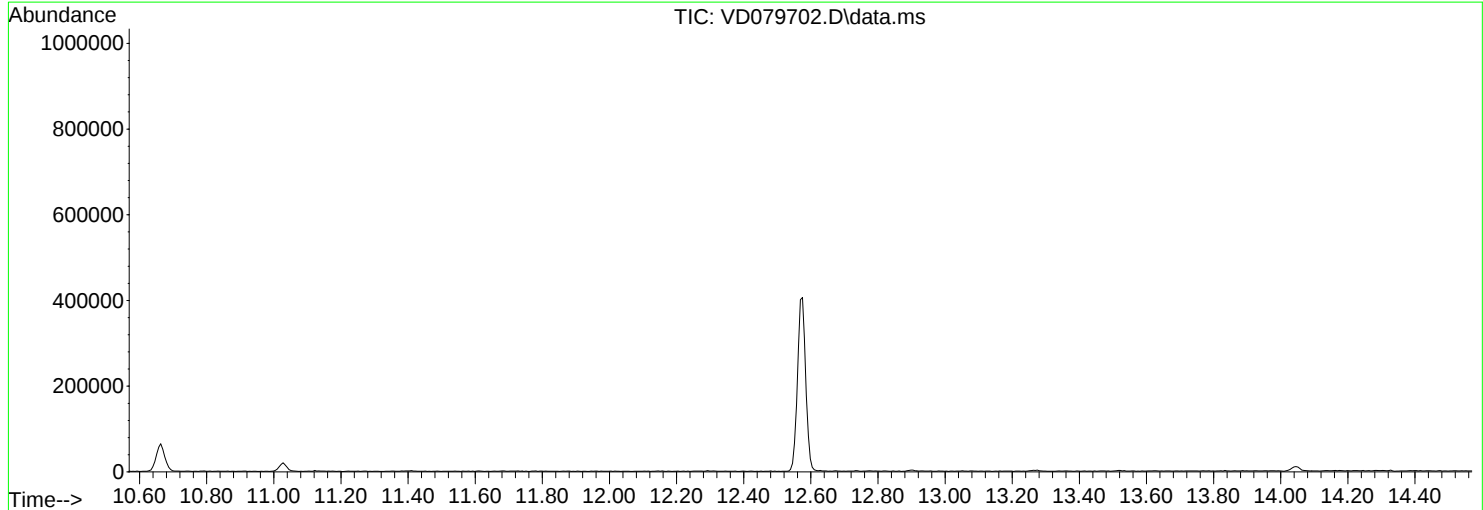

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	12800	PASS
75	95	30	60	51.6	33309	PASS
95	95	100	100	100.0	64595	PASS
96	95	5	9	7.0	4501	PASS
173	174	0.00	2	1.6	889	PASS
174	95	50	100	85.8	55403	PASS
175	174	5	9	7.6	4209	PASS
176	174	95	101	96.7	53560	PASS
177	176	5	9	6.8	3655	PASS