


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082021\
 Data File : VD070194.D
 Acq On : 20 Aug 2021 09:41
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D081321S.M
 Title : SW846 8260
 Last Update : Sat Aug 14 02:33:51 2021

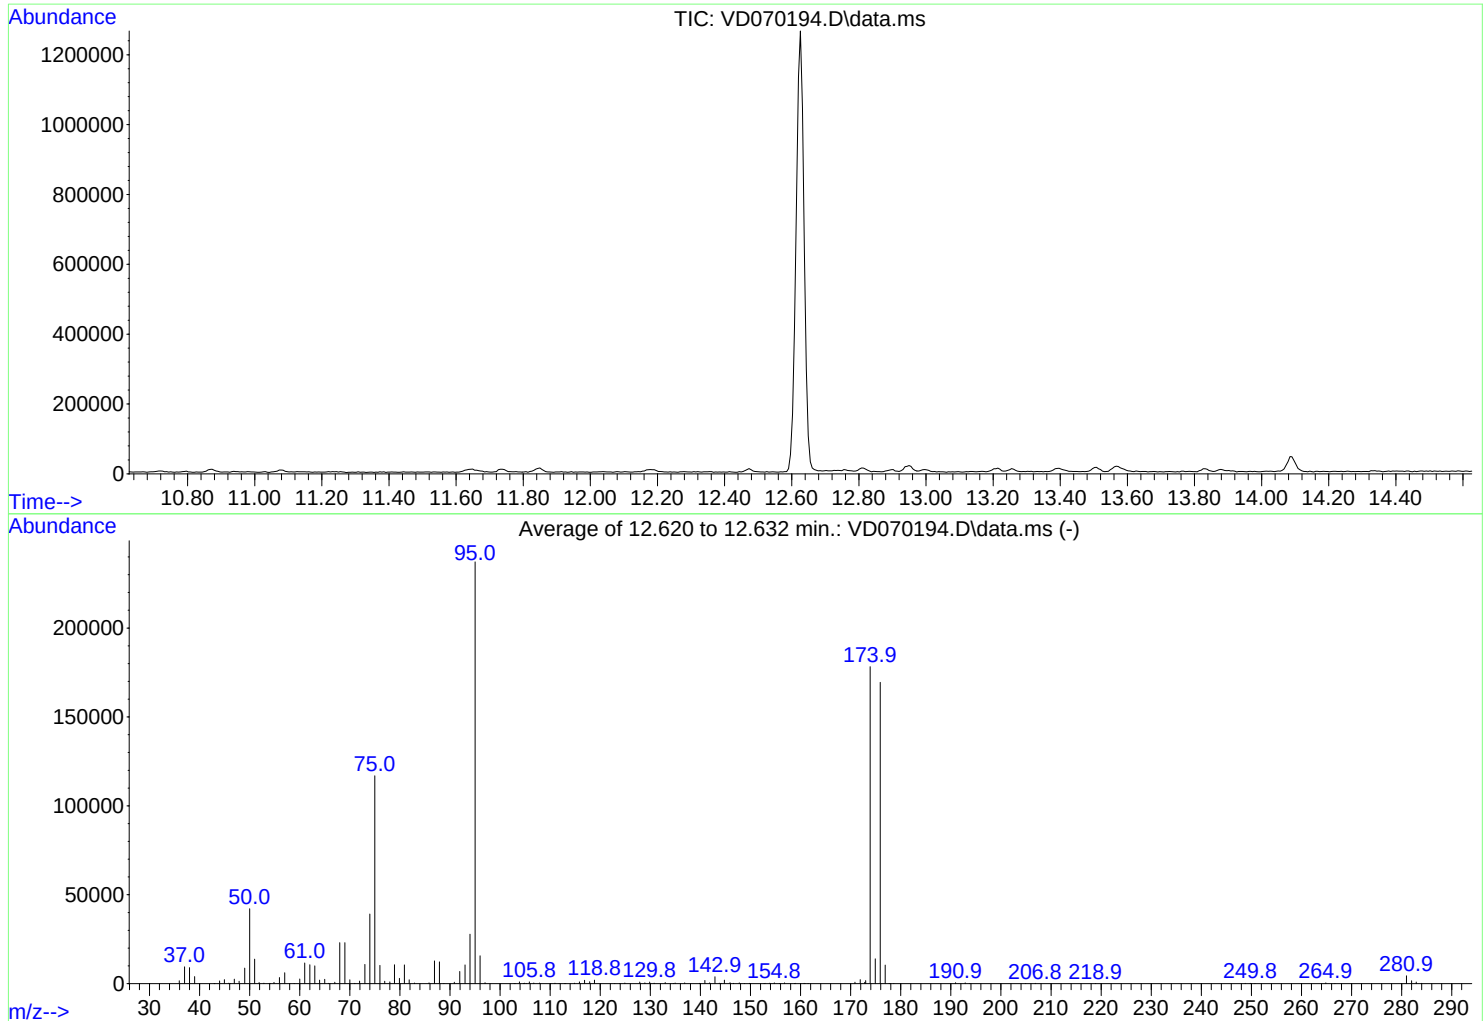

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	42136	PASS
75	95	30	60	49.3	116909	PASS
95	95	100	100	100.0	237227	PASS
96	95	5	9	6.6	15662	PASS
173	174	0.00	2	1.0	1694	PASS
174	95	50	100	75.1	178240	PASS
175	174	5	9	7.8	13983	PASS
176	174	95	101	95.1	169493	PASS
177	176	5	9	6.2	10431	PASS