

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082422\
 Data File : VD074225.D
 Acq On : 24 Aug 2022 16:06
 Operator : VA/SY
 Sample : N4272-03
 Misc : 5.03G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PSC-124055

Quant Time: Aug 24 16:35:33 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 23 13:12:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.967	168	179565	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	315508	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	281161	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.555	152	117183	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	96271	52.467	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	104.940%
35) Dibromofluoromethane	7.903	113	99168	46.990	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.980%
50) Toluene-d8	10.332	98	338387	49.821	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	99.640%
62) 4-Bromofluorobenzene	12.620	95	104364	38.895	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	77.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082422\
Data File : VD074225.D
Acq On : 24 Aug 2022 16:06
Operator : VA/SY
Sample : N4272-03
Misc : 5.03G/5.00ml/MSVOA_D/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PSC-124055

Quant Time: Aug 24 16:35:33 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 23 13:12:17 2022
Response via : Initial Calibration




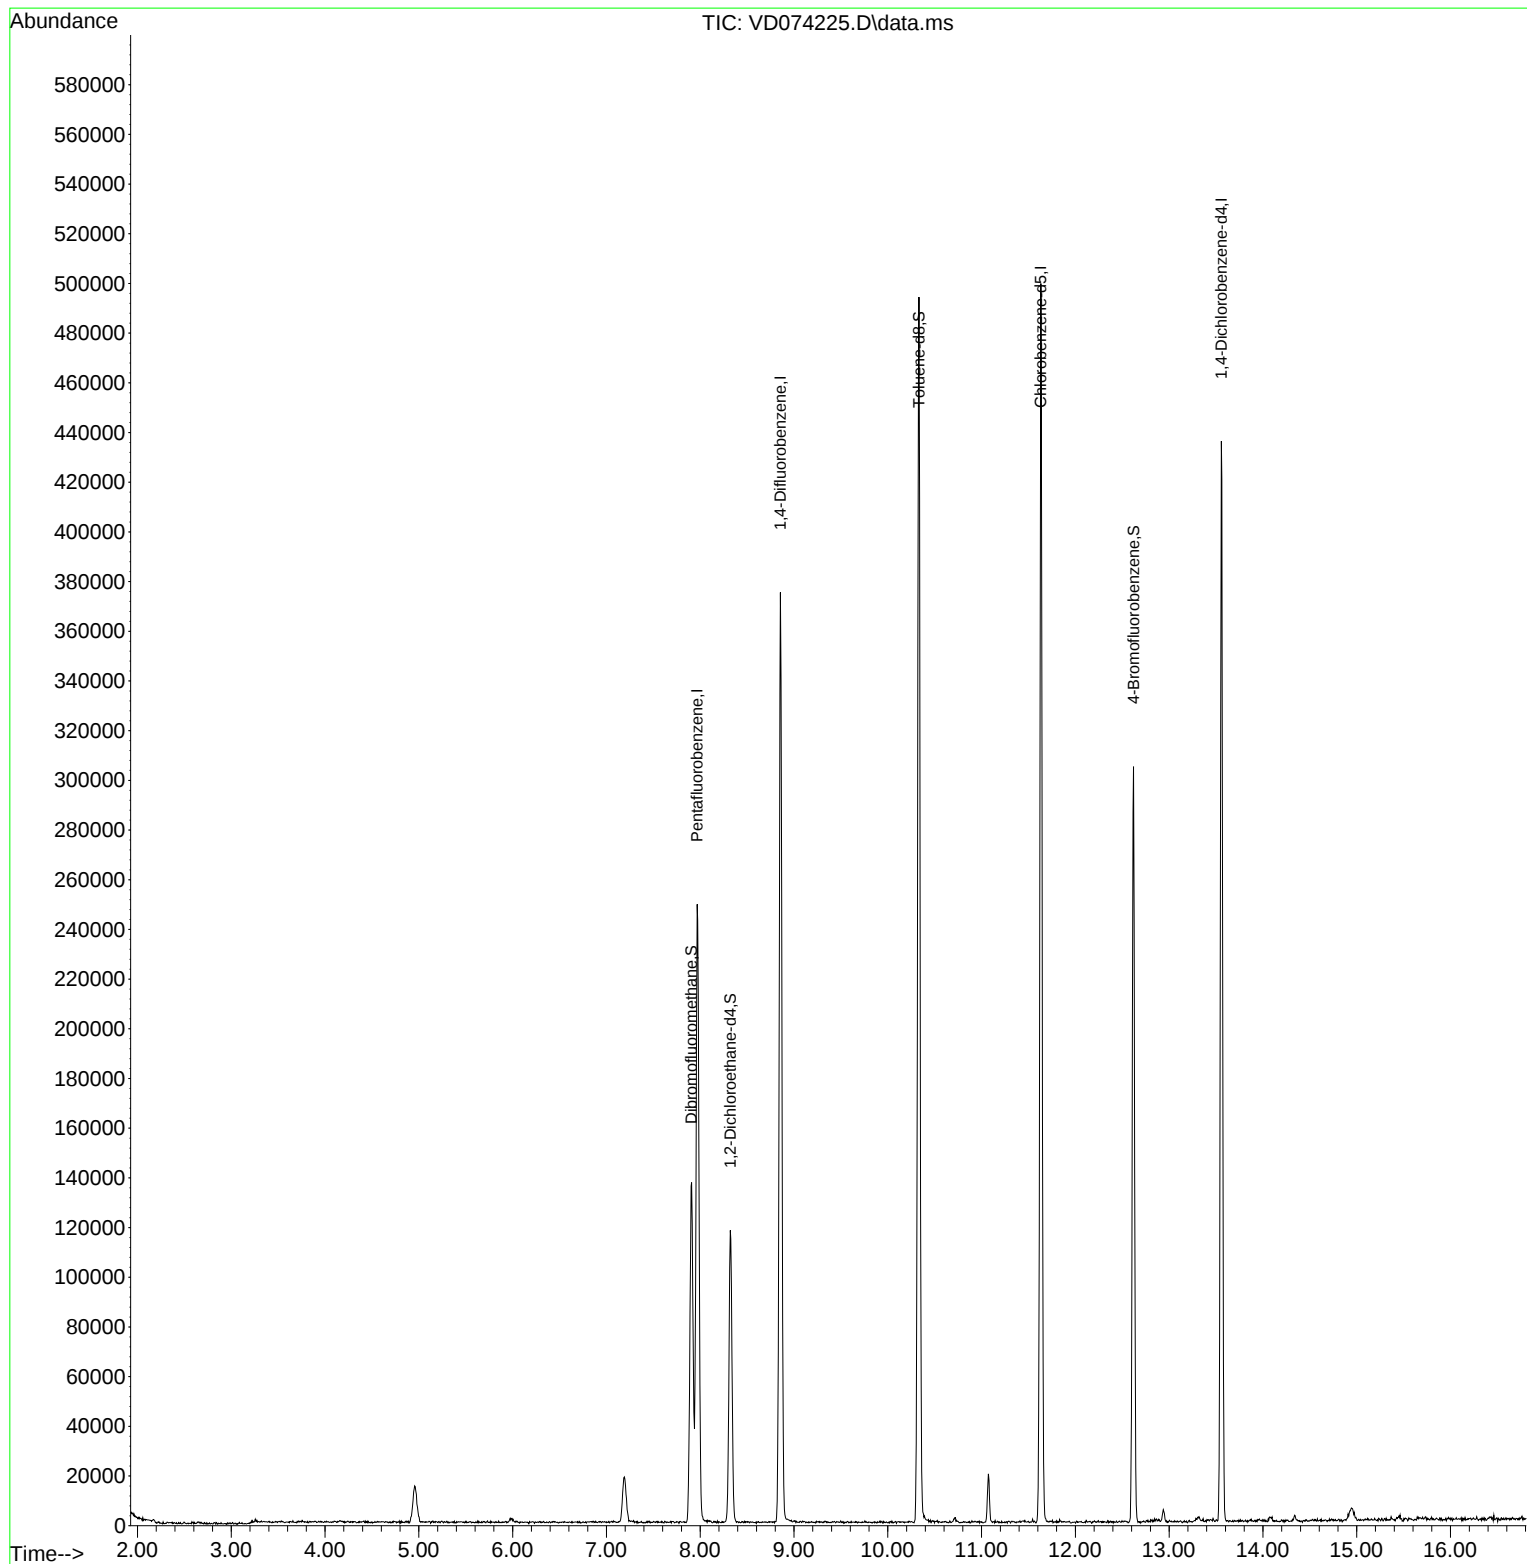


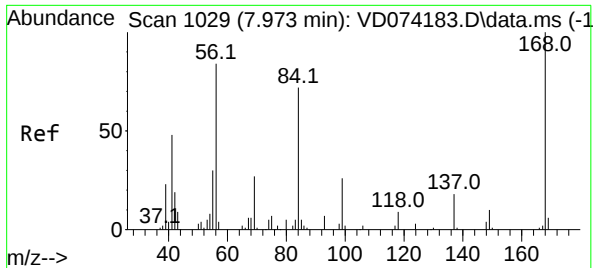

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.967 min Scan# 1028
Delta R.T. -0.006 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06




Instrument :
MSVOA_D
ClientSampleId :
PSC-124055


Tgt Ion:168 Resp: 179565
Ion Ratio Lower Upper
168 100
99 62.8 49.8 74.6

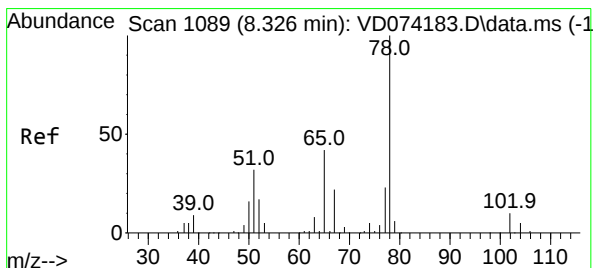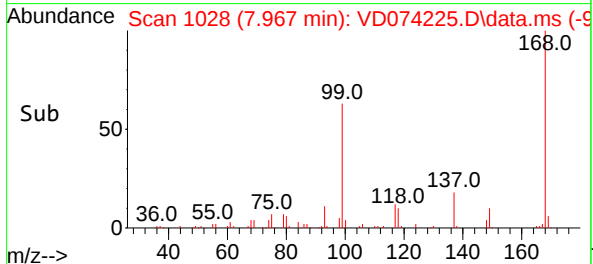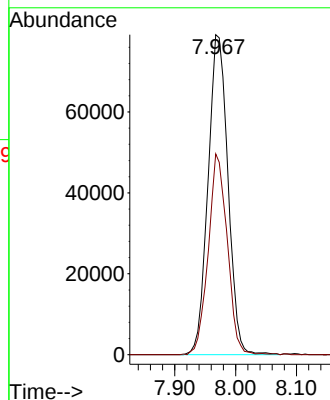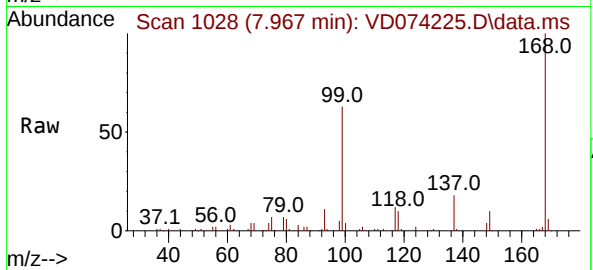

#33
1,2-Dichloroethane-d4
Concen: 52.467 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. -0.006 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06

Tgt Ion: 65 Resp: 96271
Ion Ratio Lower Upper
65 100
67 51.7 0.0 101.4

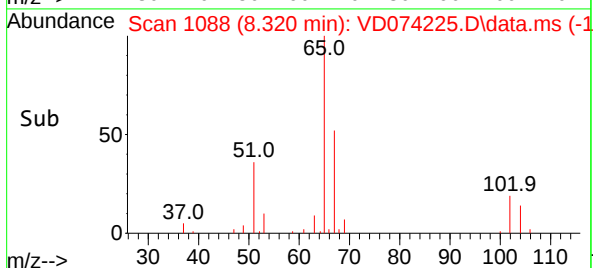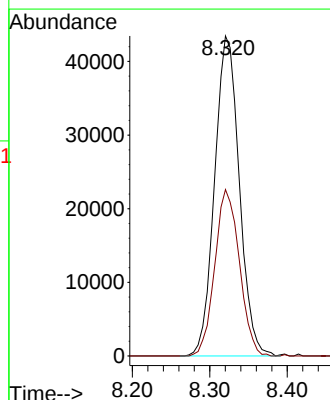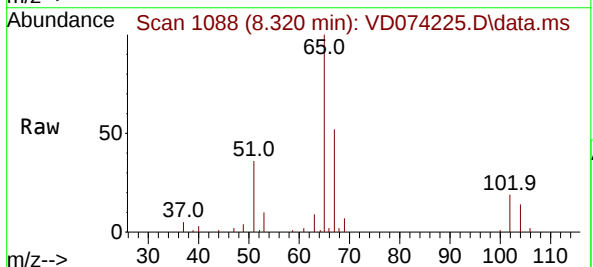

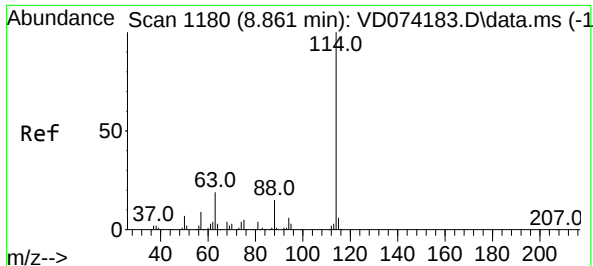

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1180

Delta R.T. -0.006 min

Lab File: VD074225.D

Acq: 24 Aug 2022 16:06

Instrument :

MSVOA_D

ClientSampleId :

PSC-124055





Tgt Ion:114 Resp: 315508

Ion Ratio Lower Upper

114 100

63 20.3 0.0 46.6

88 15.4 0.0 33.2

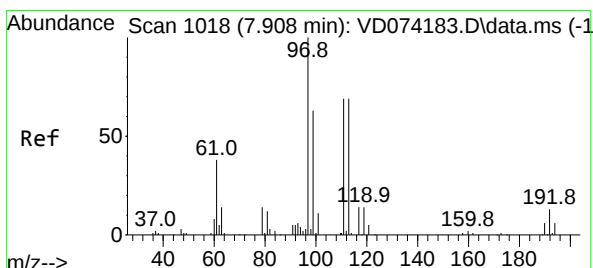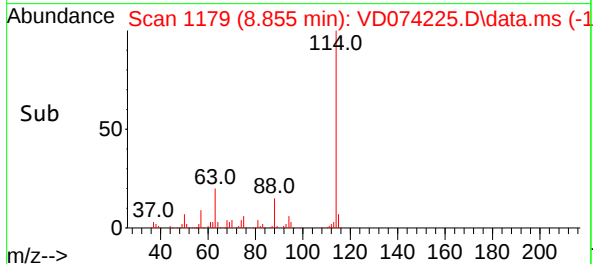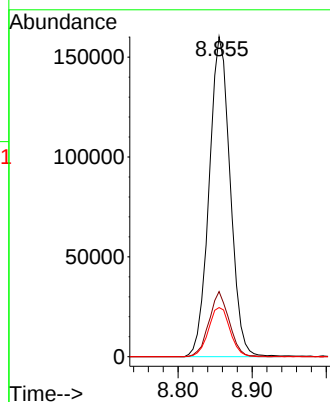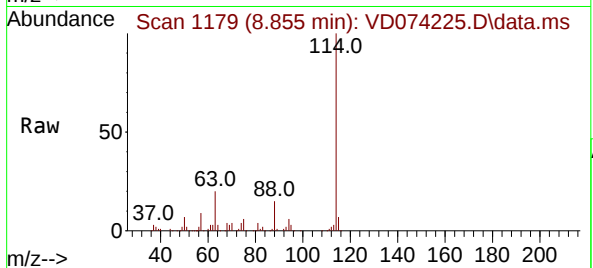

#35

Dibromofluoromethane

Concen: 46.990 ug/l

RT: 7.903 min Scan# 1017

Delta R.T. -0.005 min

Lab File: VD074225.D

Acq: 24 Aug 2022 16:06




Tgt Ion:113 Resp: 99168


Ion Ratio Lower Upper

113 100

111 102.2 83.8 125.6

192 17.8 14.6 21.8


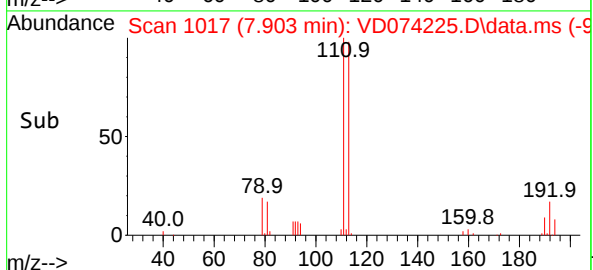
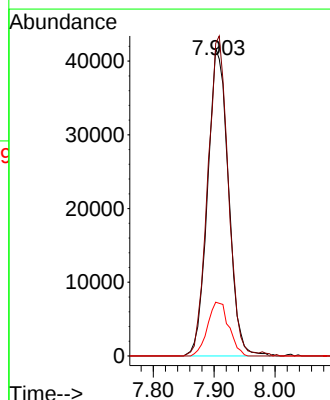
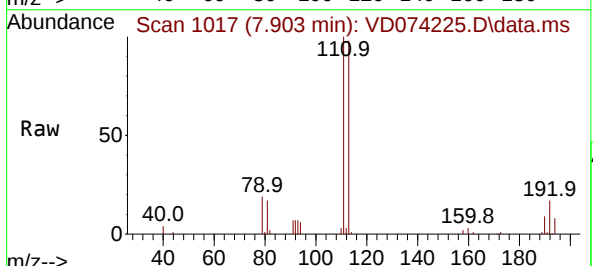


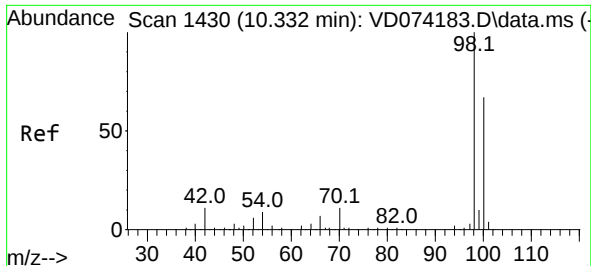

#50
Toluene-d8
Concen: 49.821 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06




Instrument :
MSVOA_D
ClientSampleId :
PSC-124055


Tgt Ion: 98 Resp: 338387
Ion Ratio Lower Upper
98 100
100 65.4 52.4 78.6

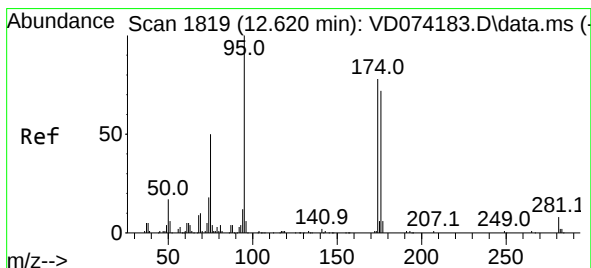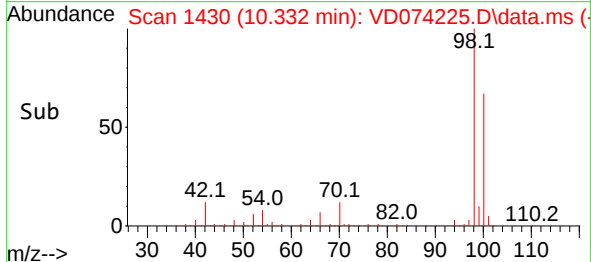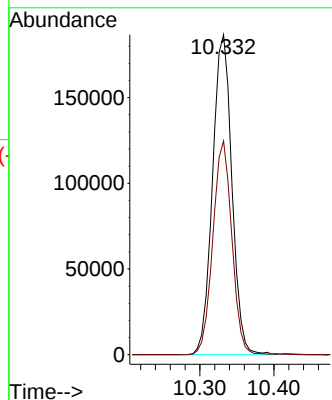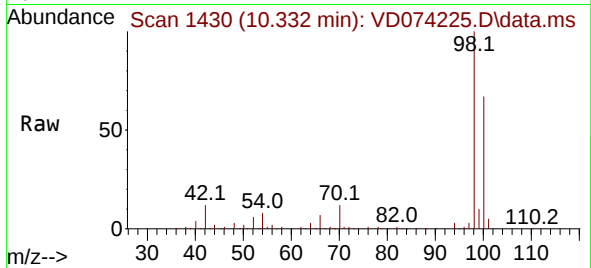

#62
4-Bromofluorobenzene
Concen: 38.895 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06

Tgt Ion: 95 Resp: 104364
Ion Ratio Lower Upper
95 100
174 77.5 0.0 152.8
176 72.6 0.0 145.4


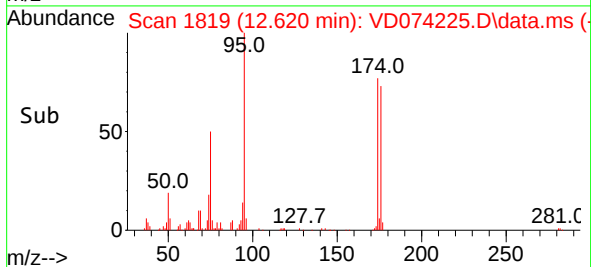
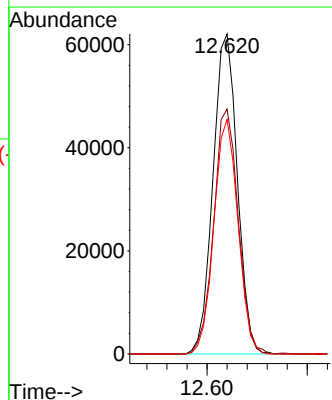
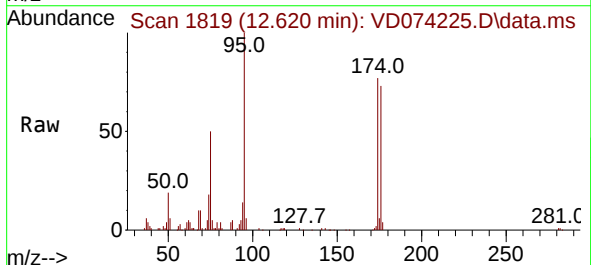


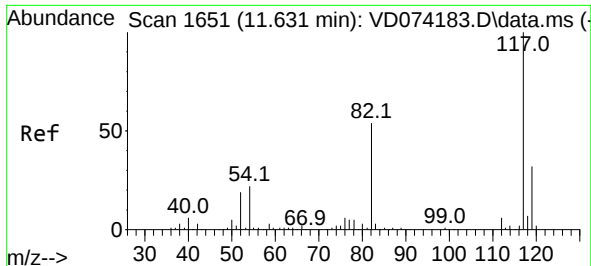

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 11
Delta R.T. 0.001 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06

Instrument :
MSVOA_D
ClientSampleId :
PSC-124055

Tgt Ion:117 Resp: 281161
Ion Ratio Lower Upper
117 100
82 54.5 45.3 67.9
119 31.5 26.6 40.0

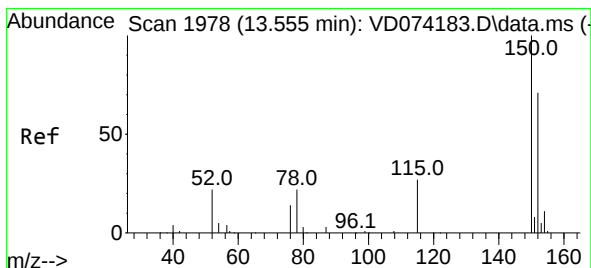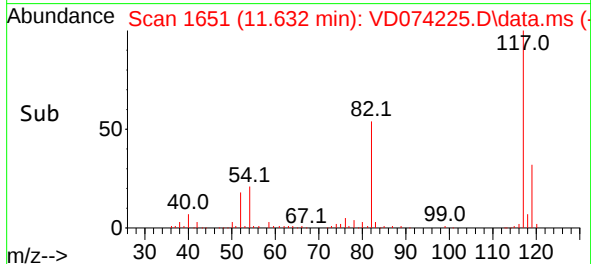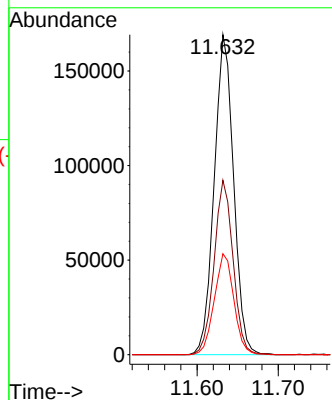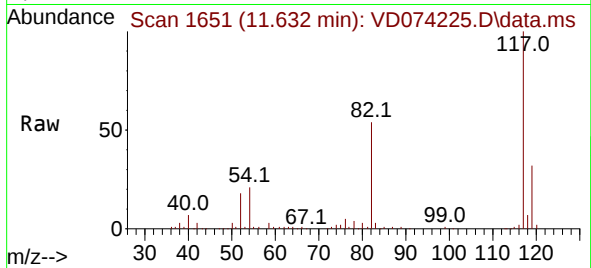

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.555 min Scan# 1978
Delta R.T. 0.000 min
Lab File: VD074225.D
Acq: 24 Aug 2022 16:06

Tgt Ion:152 Resp: 117183
Ion Ratio Lower Upper
152 100
115 60.2 31.3 93.8
150 157.1 0.0 348.6

