

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082422\
 Data File : VD074228.D
 Acq On : 24 Aug 2022 17:34
 Operator : VA/SY
 Sample : N4261-01
 Misc : 5.92G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C5

Quant Time: Aug 25 05:03:17 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 23 13:12:17 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.967	168	189349	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	343601	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	299541	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	106658	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.320	65	109952	56.827	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	113.660%
35) Dibromofluoromethane	7.902	113	108094	47.032	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	94.060%
50) Toluene-d8	10.326	98	355873	48.111	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.220%
62) 4-Bromofluorobenzene	12.614	95	103776	35.513	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	71.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082422\
Data File : VD074228.D
Acq On : 24 Aug 2022 17:34
Operator : VA/SY
Sample : N4261-01
Misc : 5.92G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C5

Quant Time: Aug 25 05:03:17 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 23 13:12:17 2022
Response via : Initial Calibration




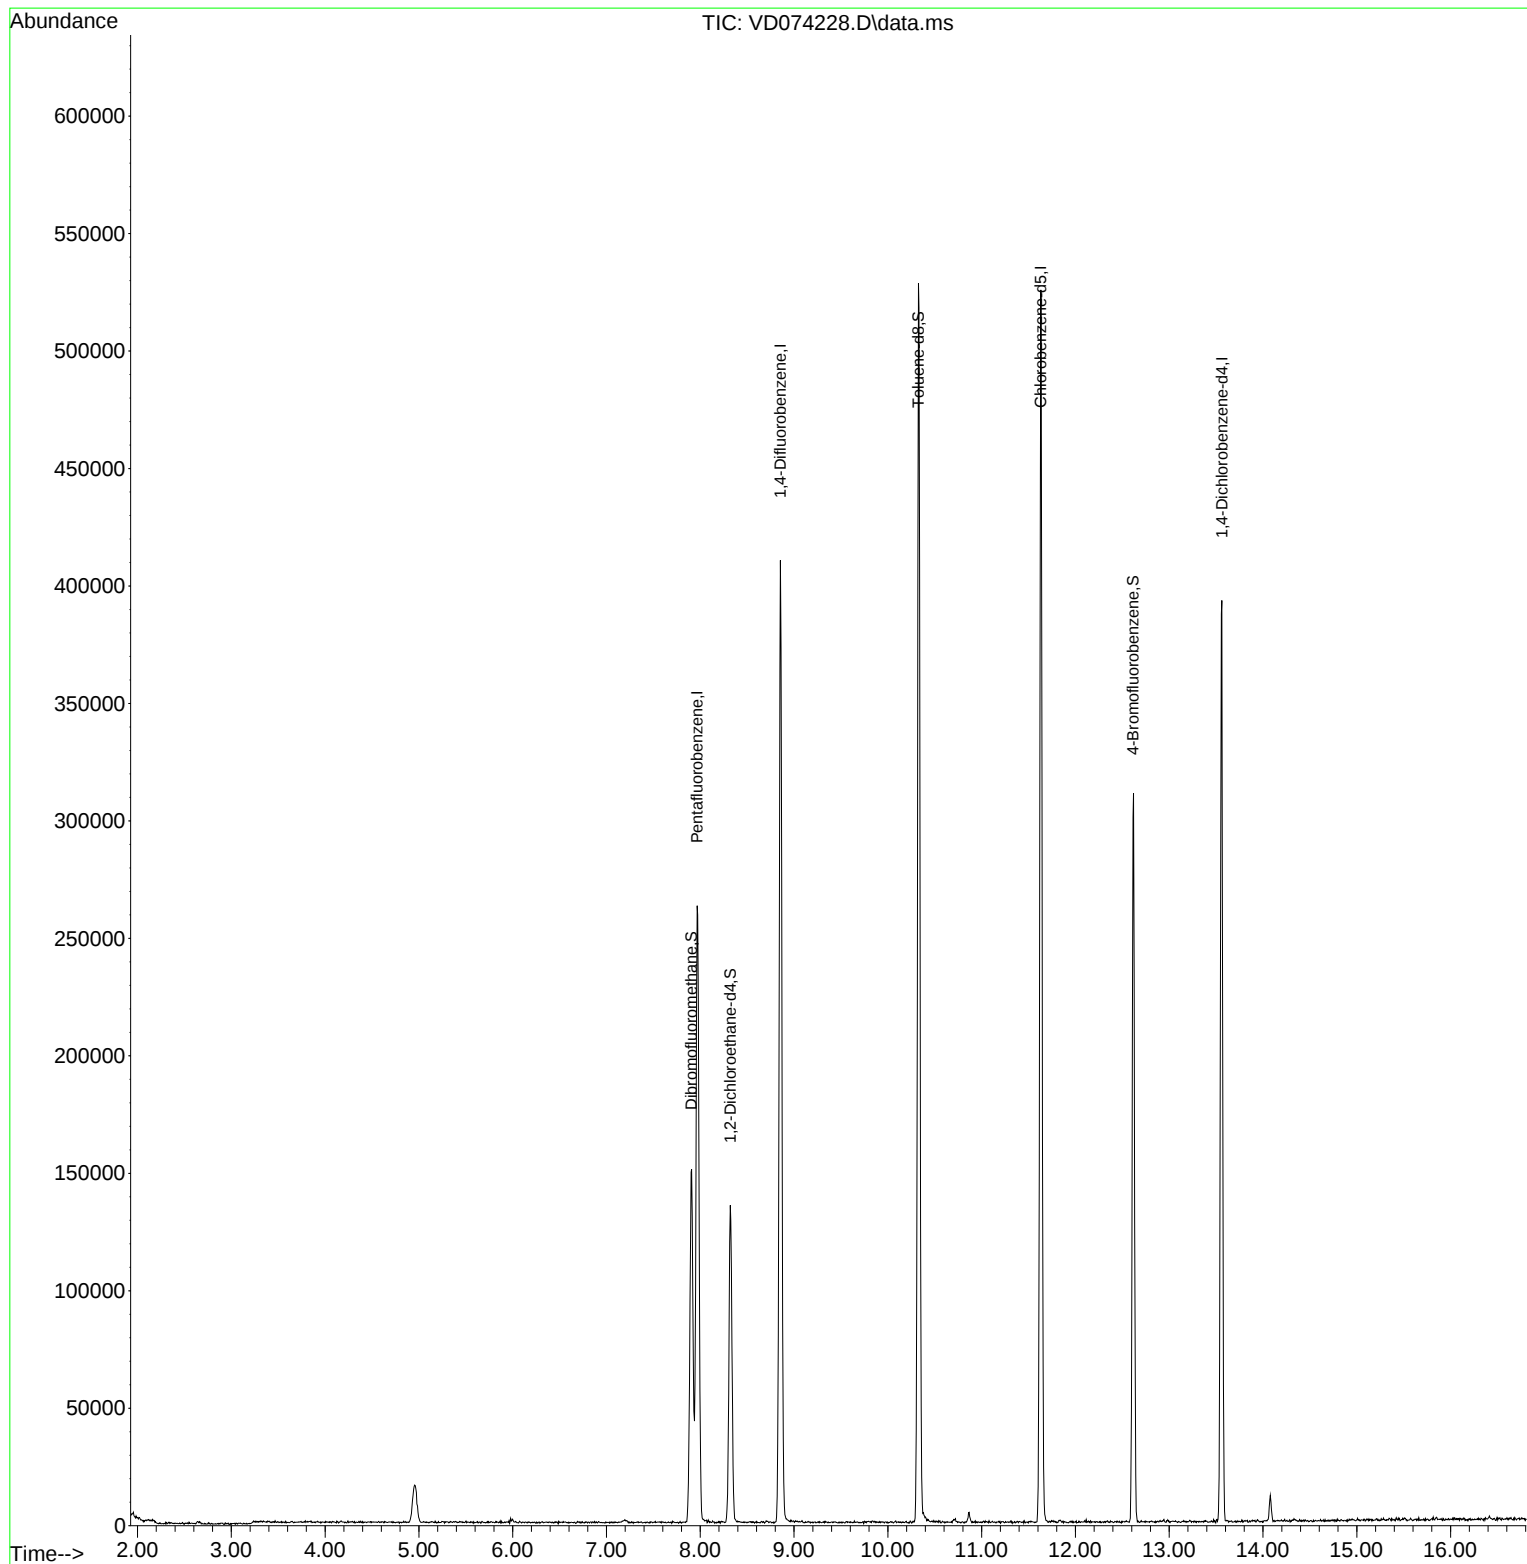


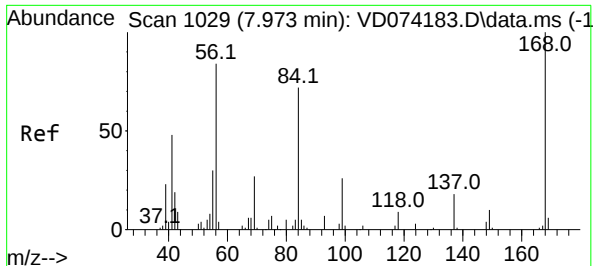

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.967 min Scan# 1028
Delta R.T. -0.006 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34




Instrument :
MSVOA_D
ClientSampleId :
C5


Tgt Ion:168 Resp: 189349
Ion Ratio Lower Upper
168 100
99 60.0 49.8 74.6

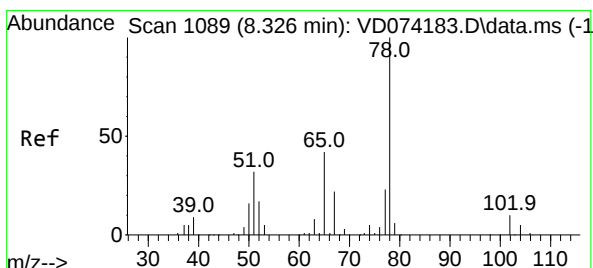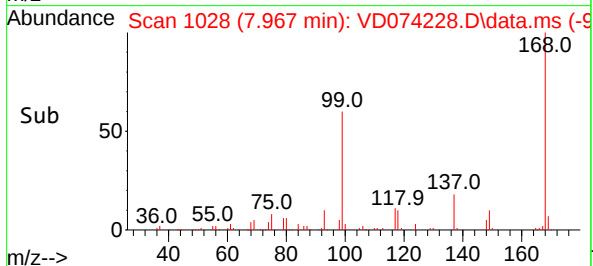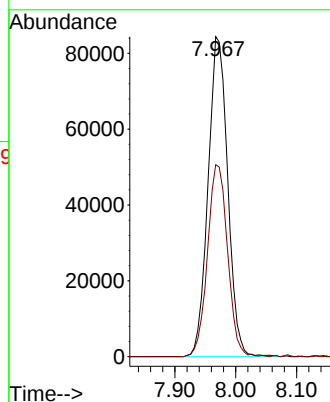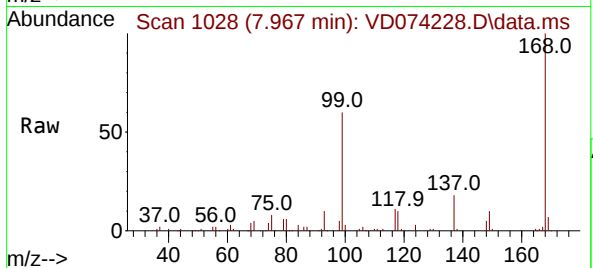

#33
1,2-Dichloroethane-d4
Concen: 56.827 ug/l
RT: 8.320 min Scan# 1088
Delta R.T. -0.006 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34

Tgt Ion: 65 Resp: 109952
Ion Ratio Lower Upper
65 100
67 52.4 0.0 101.4

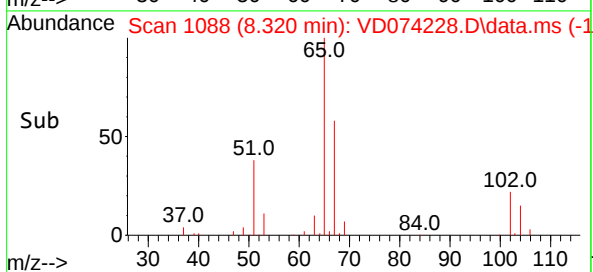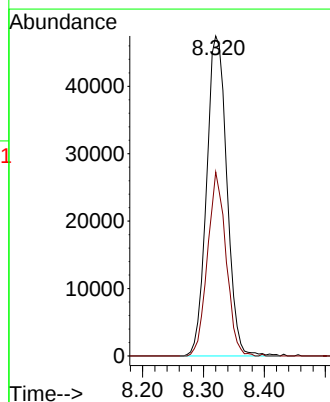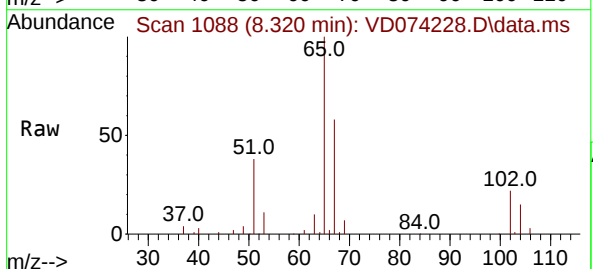

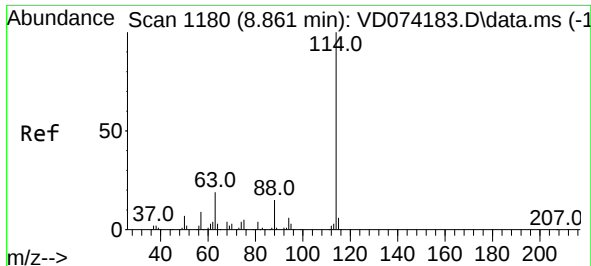

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.855 min Scan# 1179

Delta R.T. -0.006 min

Lab File: VD074228.D

Acq: 24 Aug 2022 17:34

Instrument :

MSVOA_D

ClientSampleId :

C5





Tgt Ion:114 Resp: 343601

Ion Ratio Lower Upper

114 100

63 20.7 0.0 46.6

88 15.7 0.0 33.2

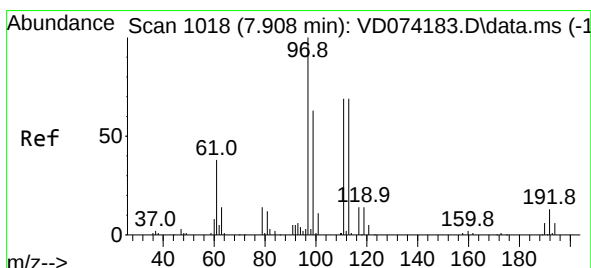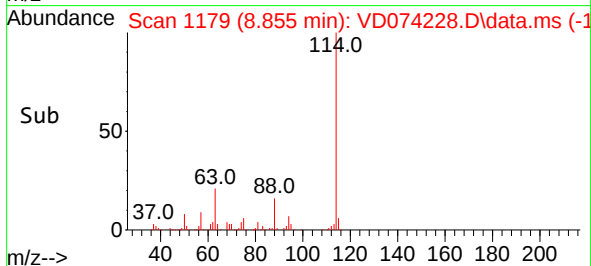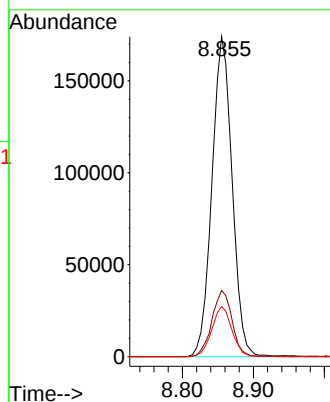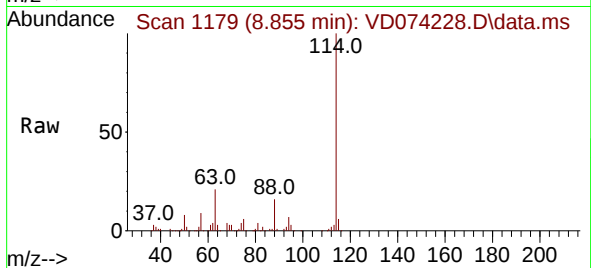

#35

Dibromofluoromethane

Concen: 47.032 ug/l

RT: 7.902 min Scan# 1017

Delta R.T. -0.006 min

Lab File: VD074228.D

Acq: 24 Aug 2022 17:34




Tgt Ion:113 Resp: 108094


Ion Ratio Lower Upper

113 100

111 103.8 83.8 125.6

192 18.7 14.6 21.8


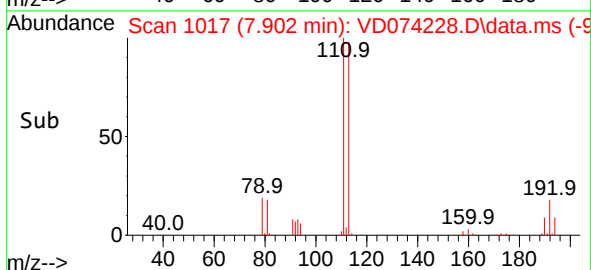
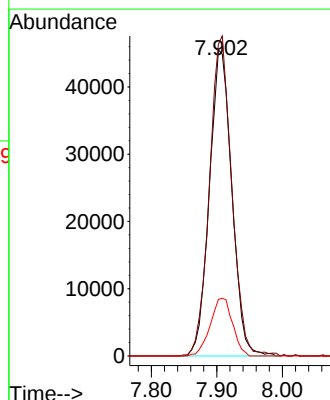
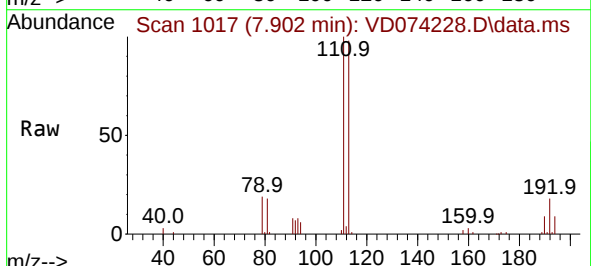


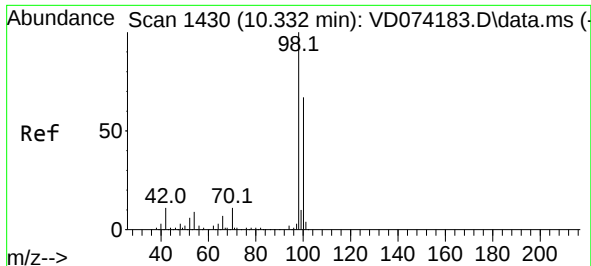

#50
Toluene-d8
Concen: 48.111 ug/l
RT: 10.326 min Scan# 1430
Delta R.T. -0.006 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34




Instrument :
MSVOA_D
ClientSampleId :
C5


Tgt Ion: 98 Resp: 355873
Ion Ratio Lower Upper
98 100
100 66.6 52.4 78.6

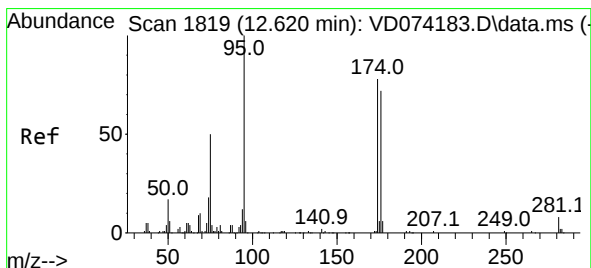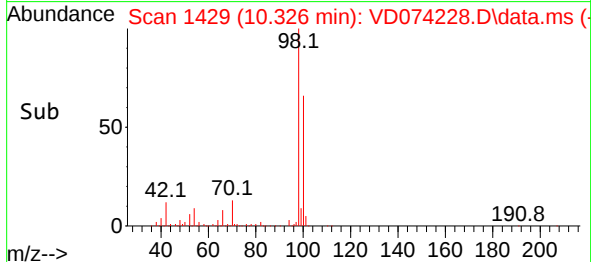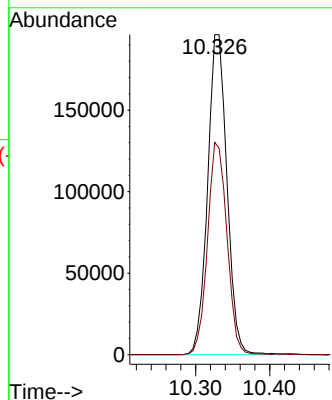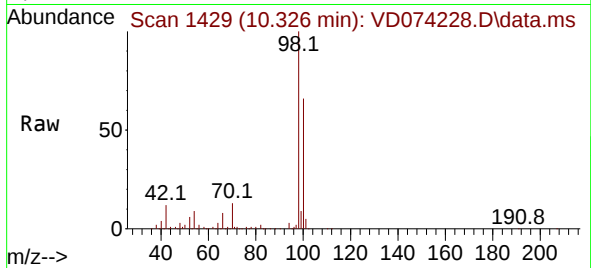

#62
4-Bromofluorobenzene
Concen: 35.513 ug/l
RT: 12.614 min Scan# 1818
Delta R.T. -0.006 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34

Tgt Ion: 95 Resp: 103776
Ion Ratio Lower Upper
95 100
174 76.0 0.0 152.8
176 72.3 0.0 145.4


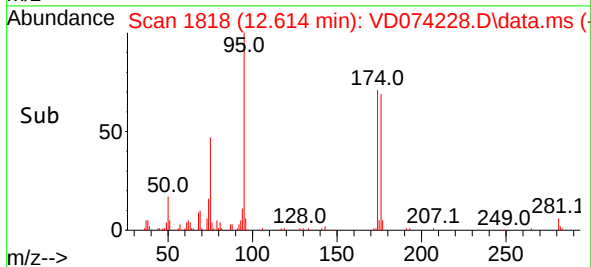
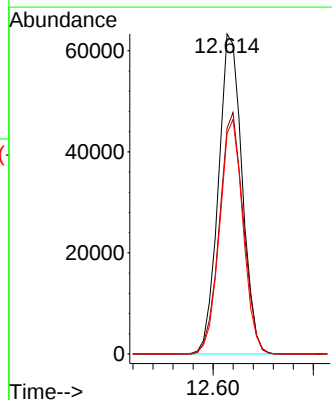
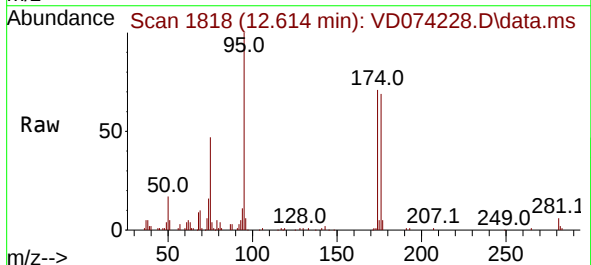


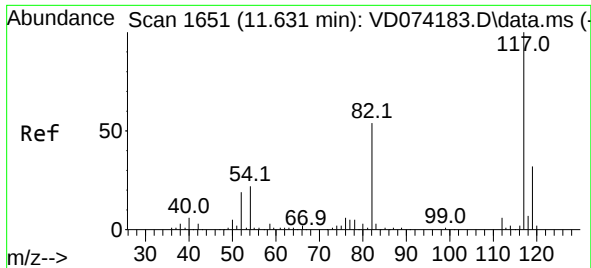

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 117
Delta R.T. 0.001 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34

Instrument :
MSVOA_D
ClientSampleId :
C5

Tgt Ion:117 Resp: 299541
Ion Ratio Lower Upper
117 100
82 54.2 45.3 67.9
119 31.5 26.6 40.0

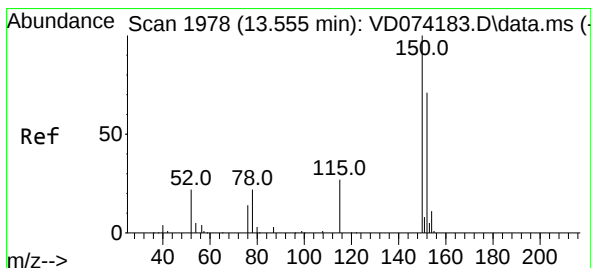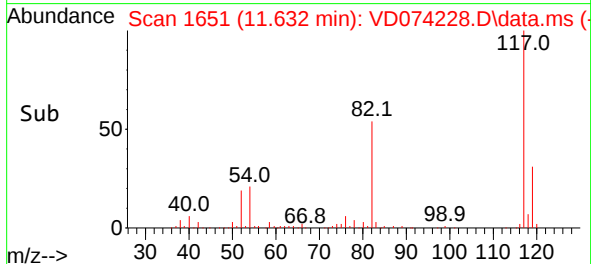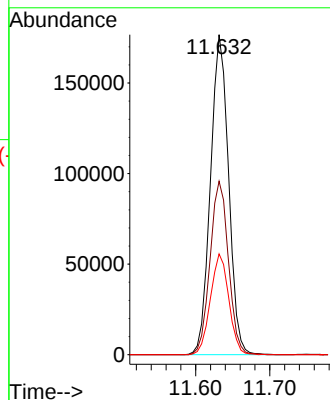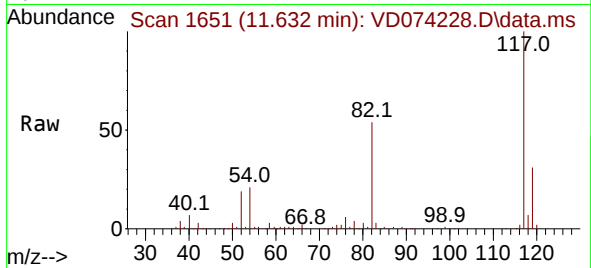

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.006 min
Lab File: VD074228.D
Acq: 24 Aug 2022 17:34

Tgt Ion:152 Resp: 106658
Ion Ratio Lower Upper
152 100
115 59.5 31.3 93.8
150 155.9 0.0 348.6

