
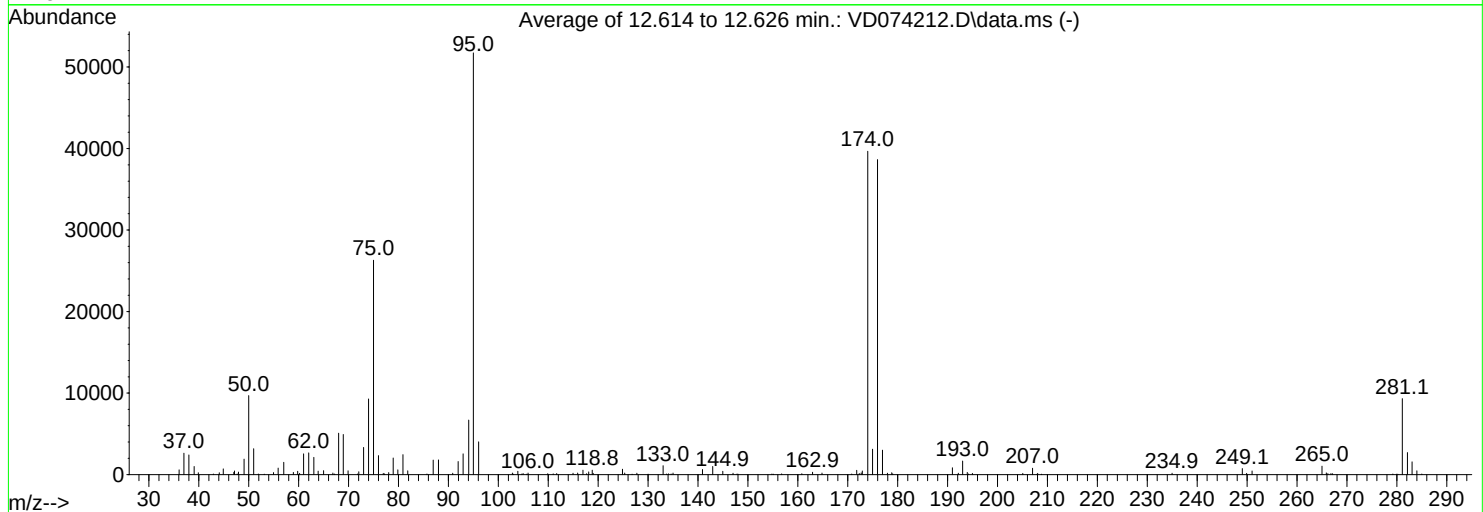


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD082422\
Data File : VD074212.D
Acq On : 24 Aug 2022 09:11
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082322S.M
Title : SW846 8260
Last Update : Tue Aug 23 13:12:17 2022

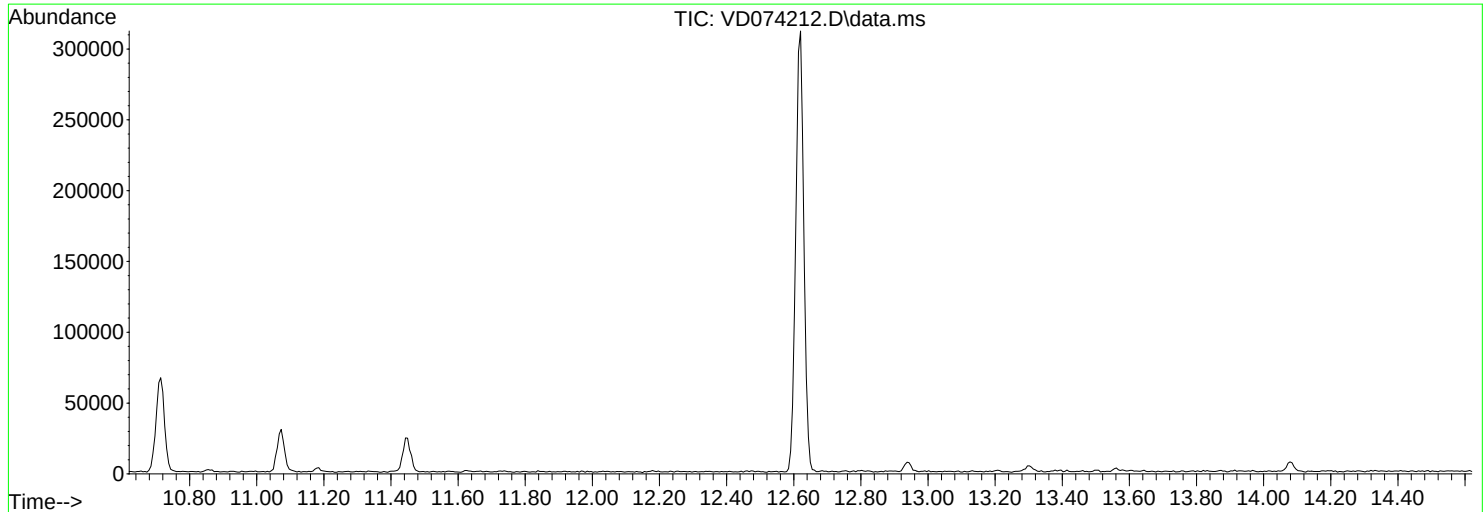

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	9687	PASS
75	95	30	60	50.8	26293	PASS
95	95	100	100	100.0	51733	PASS
96	95	5	9	7.8	4016	PASS
173	174	0.00	2	1.2	457	PASS
174	95	50	100	76.7	39669	PASS
175	174	5	9	7.9	3122	PASS
176	174	95	101	97.4	38643	PASS
177	176	5	9	7.8	3009	PASS