
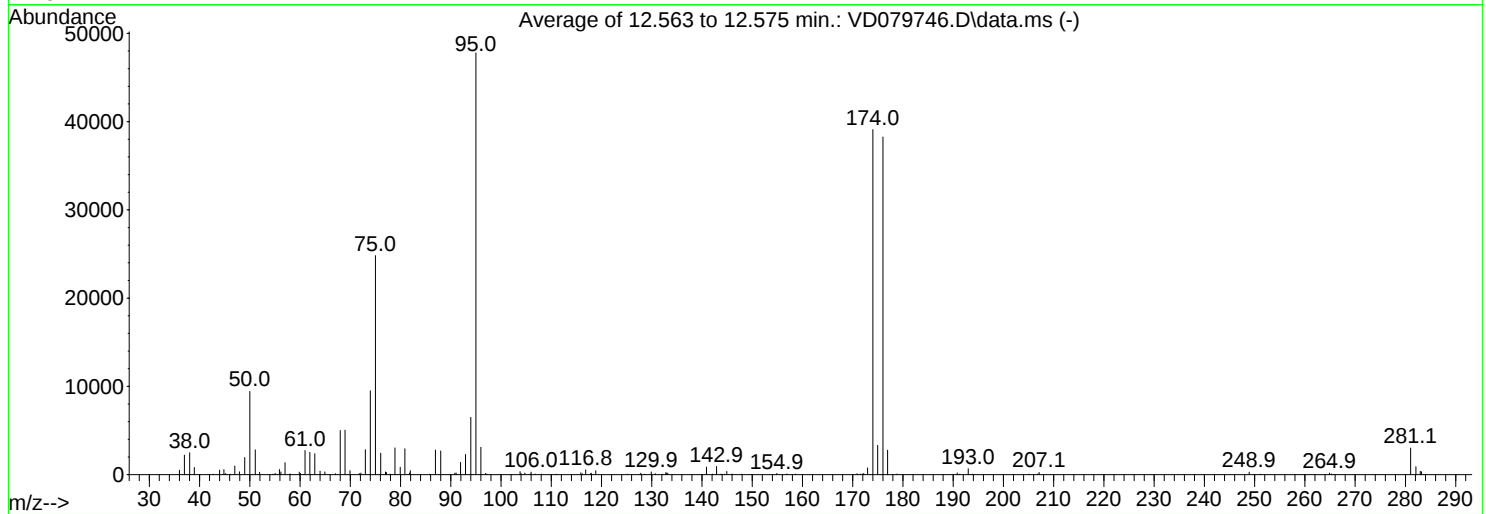


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD083024\
Data File : VD079746.D
Acq On : 30 Aug 2024 10:00
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D083024S.M
Title : SW846 8260
Last Update : Fri Aug 30 15:57:30 2024

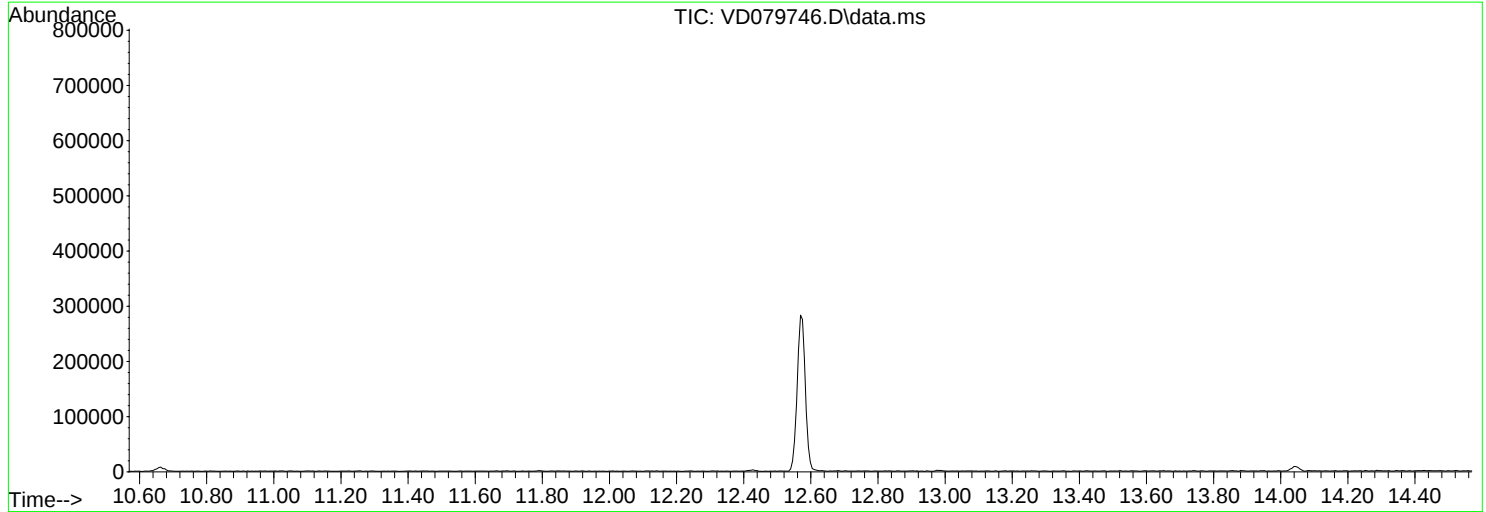

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	9428	PASS
75	95	30	60	51.9	24816	PASS
95	95	100	100	100.0	47792	PASS
96	95	5	9	6.5	3095	PASS
173	174	0.00	2	1.9	761	PASS
174	95	50	100	81.8	39099	PASS
175	174	5	9	8.5	3320	PASS
176	174	95	101	97.8	38253	PASS
177	176	5	9	7.3	2775	PASS