
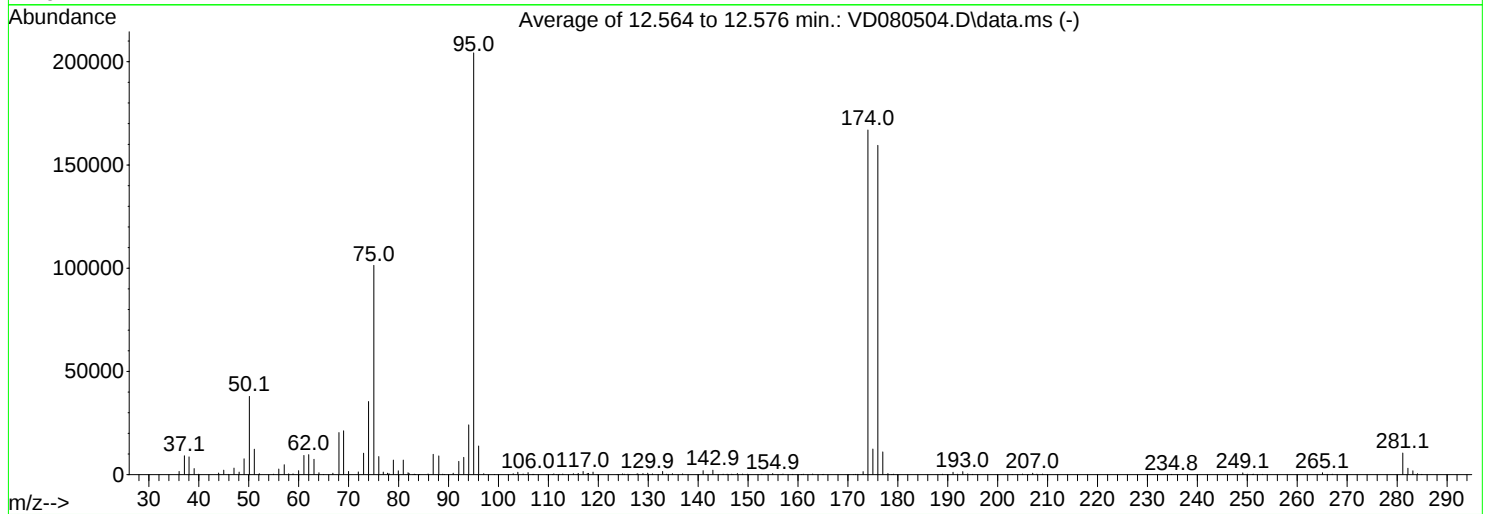


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080504\
Data File : VD080504.D
Acq On : 04 Sep 2025 08:27
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082725S.M
Title : SW846 8260
Last Update : Thu Aug 28 03:02:37 2025

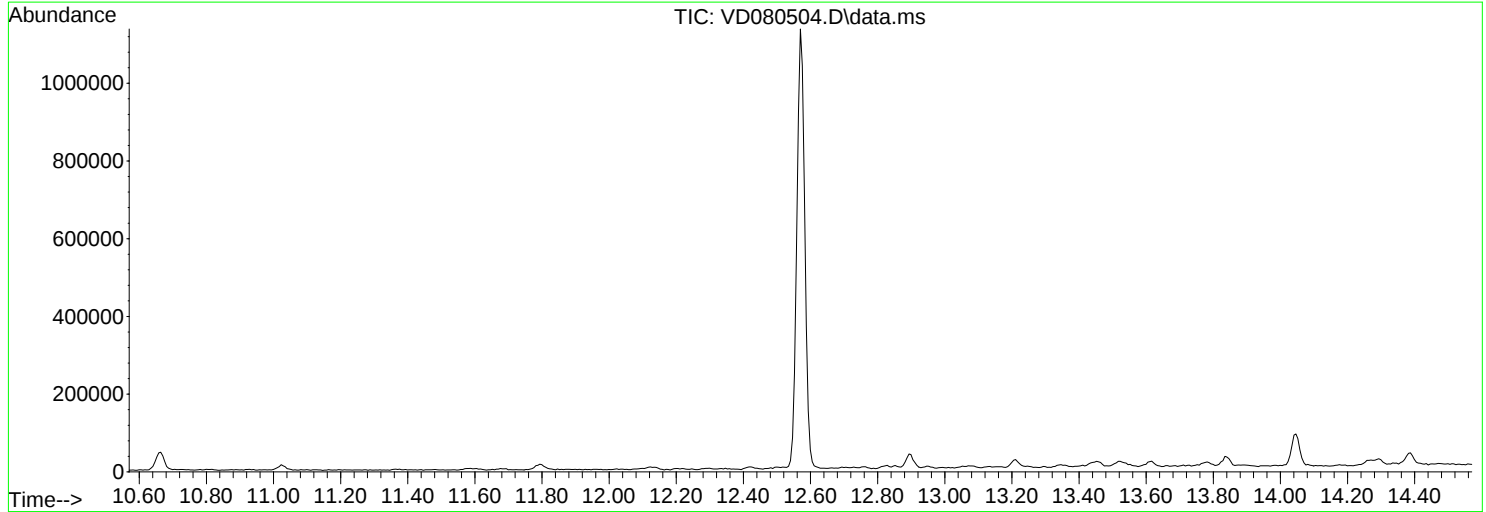

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	37925	PASS
75	95	30	60	49.6	101344	PASS
95	95	100	100	100.0	204309	PASS
96	95	5	9	6.8	13875	PASS
173	174	0.00	2	0.9	1468	PASS
174	95	50	100	81.7	166955	PASS
175	174	5	9	7.4	12391	PASS
176	174	95	101	95.5	159509	PASS
177	176	5	9	6.9	11027	PASS