

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090525\
 Data File : VD080515.D
 Acq On : 05 Sep 2025 09:54
 Operator : RP/MD
 Sample : VD0905SBL01
 Misc : 5.00G/5ml/MSVOA_D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :

Quant Time: Sep 06 02:59:19 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082725S.M
 Quant Title : SW846 8260
 QLast Update : Thu Aug 28 03:02:37 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.876	168	361670	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.776	114	625107	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.582	117	541756	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.517	152	254170	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.229	65	184017	45.098	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery =	90.200%		
35) Dibromofluoromethane	7.805	113	179913	47.418	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery =	94.840%		
50) Toluene-d8	10.270	98	730749	48.549	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery =	97.100%		
62) 4-Bromofluorobenzene	12.570	95	222177	46.781	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery =	93.560%		
Target Compounds						
					Qvalue	
13) Acrolein	3.794	56	430	1.370	ug/l #	60
16) Acetone	4.017	43	1122	1.175	ug/l #	43
31) Cyclohexane	7.876	56	8437	1.104	ug/l #	17
38) Carbon Tetrachloride	7.876	117	34876	6.689	ug/l #	13
76) 1,2,3-Trichloropropane	12.570	75	113138	54.540	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.570	75	113138	82.779	ug/l #	19


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD090525\
Data File : VD080515.D
Acq On : 05 Sep 2025 09:54
Operator : RP/MD
Sample : VD0905SBL01
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :

Quant Time: Sep 06 02:59:19 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082725S.M
Quant Title : SW846 8260
QLast Update : Thu Aug 28 03:02:37 2025
Response via : Initial Calibration




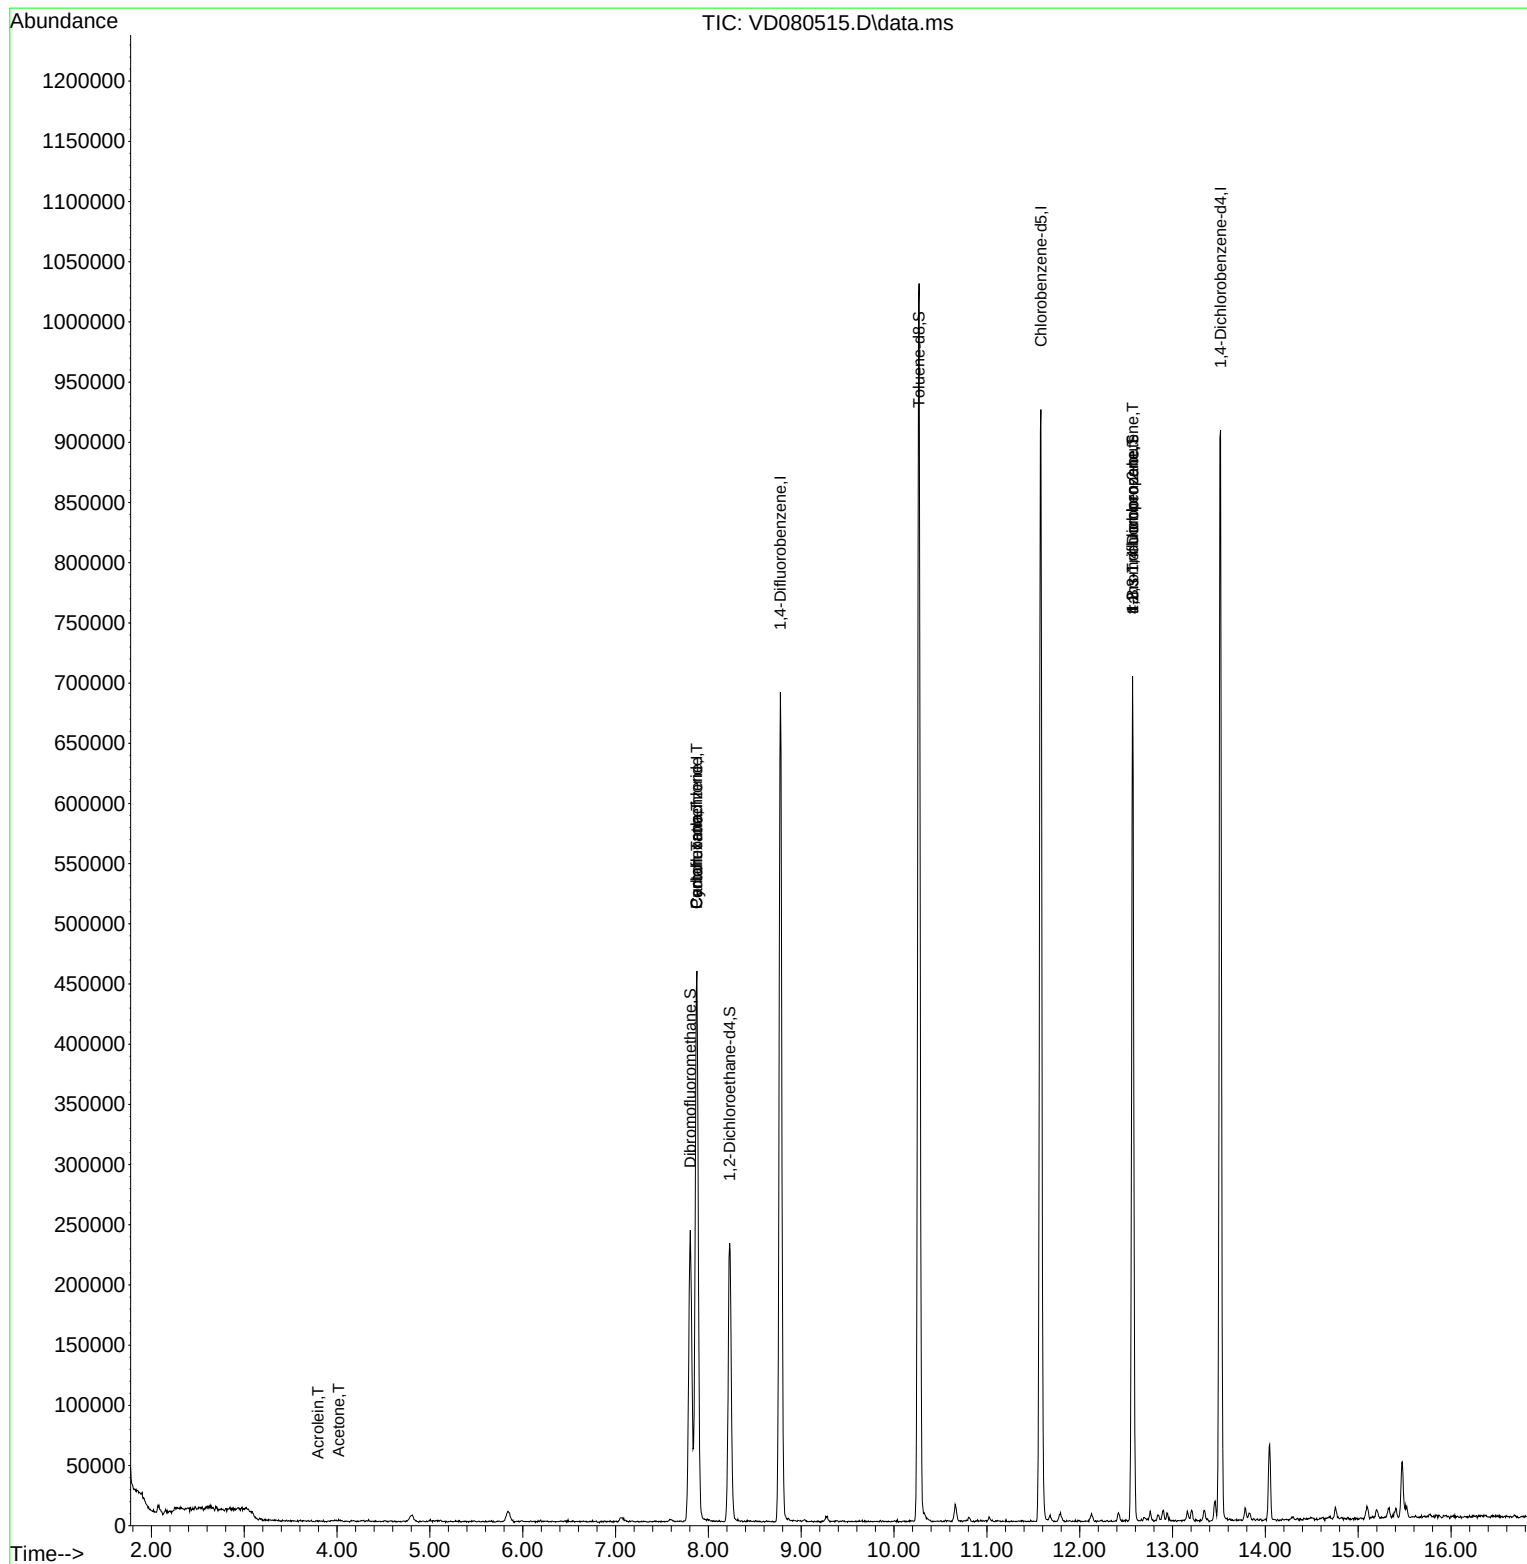


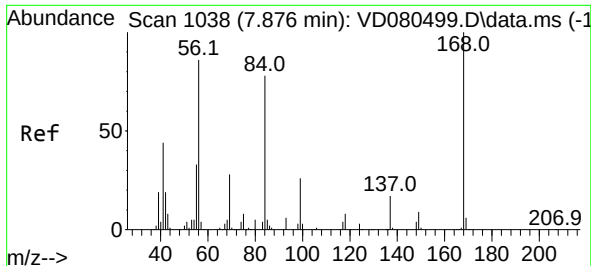

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.876 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion:168 Resp: 361670
Ion Ratio Lower Upper
168 100
99 54.5 44.1 66.1

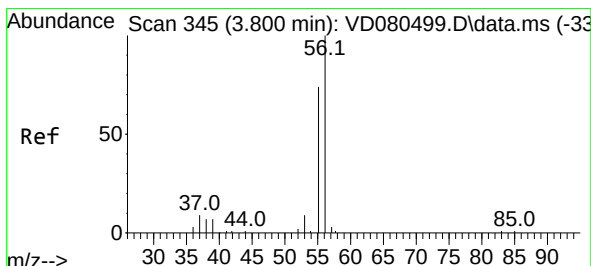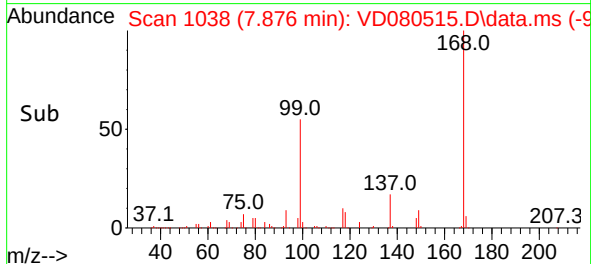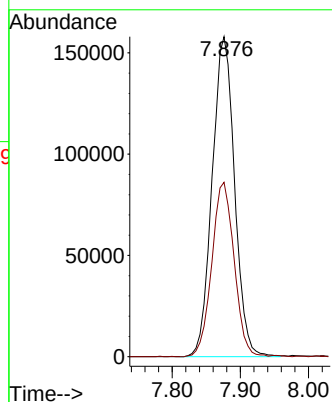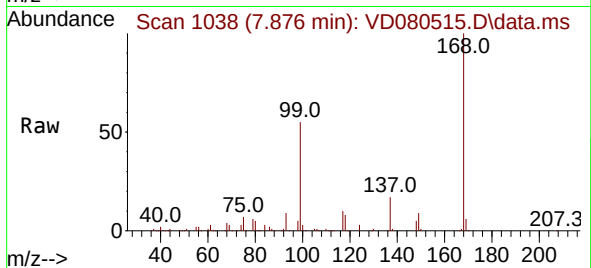

#13
Acrolein
Concen: 1.370 ug/l
RT: 3.794 min Scan# 344
Delta R.T. -0.006 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54

Tgt Ion: 56 Resp: 430
Ion Ratio Lower Upper
56 100
55 37.4 56.6 85.0#


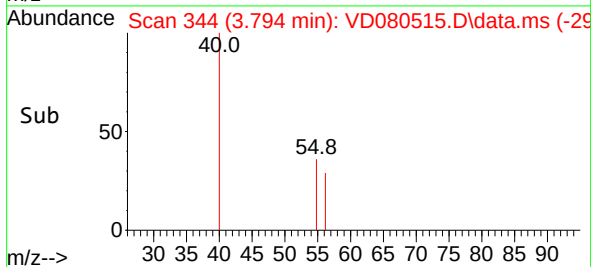
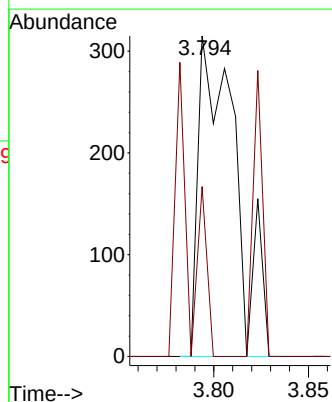
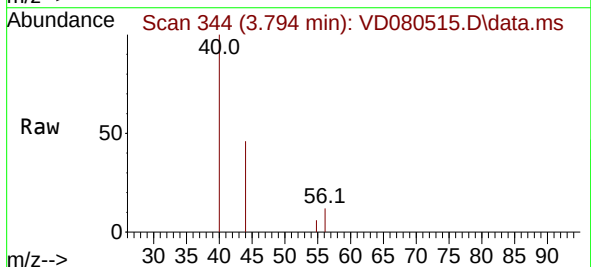


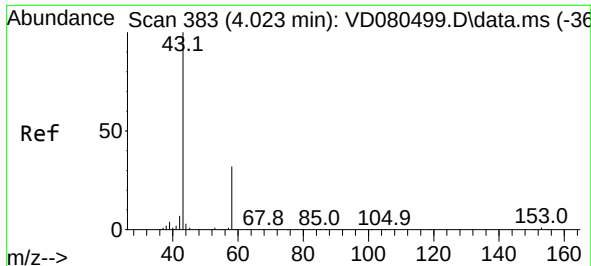

#16
Acetone
Concen: 1.175 ug/l
RT: 4.017 min Scan# 382
Delta R.T. -0.006 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 43 Resp: 1122
Ion Ratio Lower Upper
43 100
58 0.0 25.4 38.0#

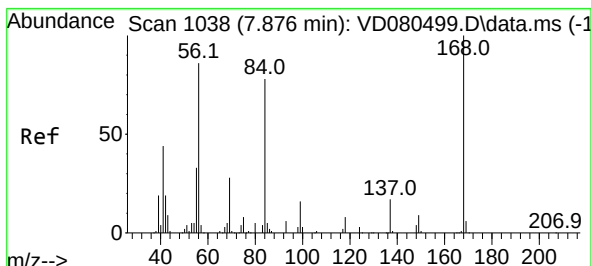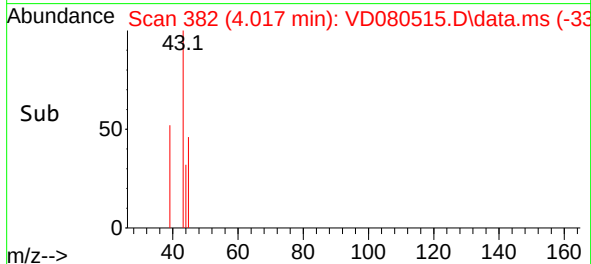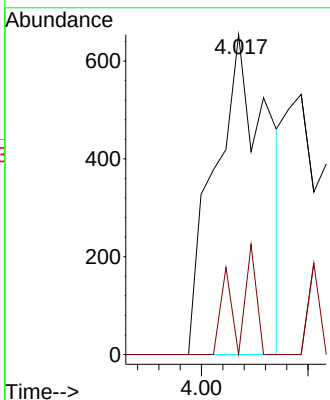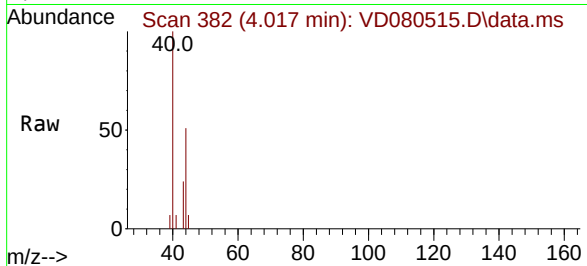

#31
Cyclohexane
Concen: 1.104 ug/l
RT: 7.876 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54

Tgt Ion: 56 Resp: 8437
Ion Ratio Lower Upper
56 100
69 134.3 26.0 39.0#
84 136.1 72.6 108.8#

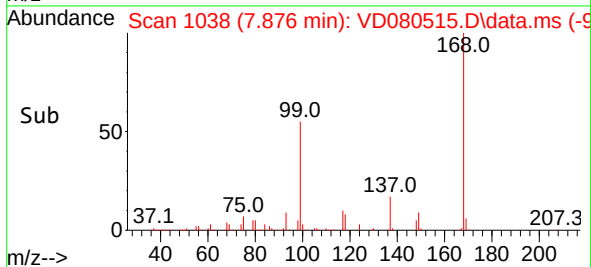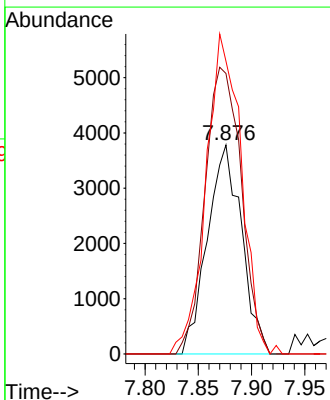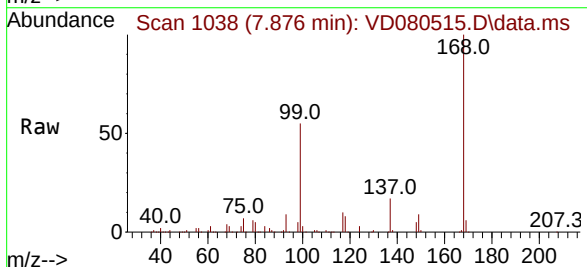

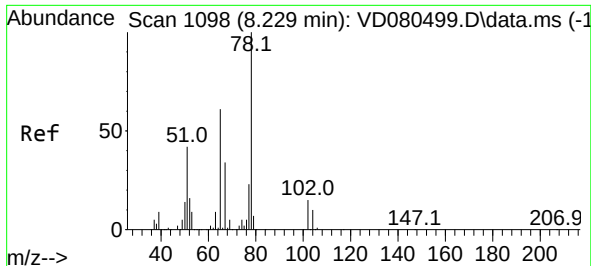

#33

1,2-Dichloroethane-d4

Concen: 45.098 ug/l

RT: 8.229 min Scan# 1098

Delta R.T. -0.000 min

Lab File: VD080515.D

Acq: 05 Sep 2025 09:54

Instrument :

MSVOA_D





ClientSampleId :

Tgt Ion: 65 Resp: 184017

Ion Ratio Lower Upper

65 100

67 53.3 0.0 113.0

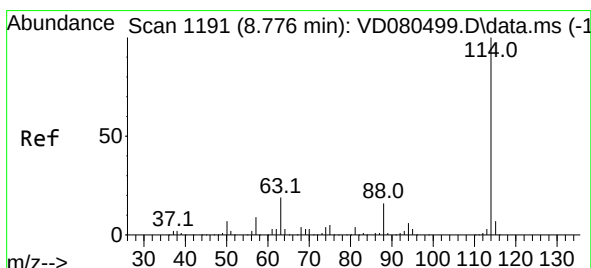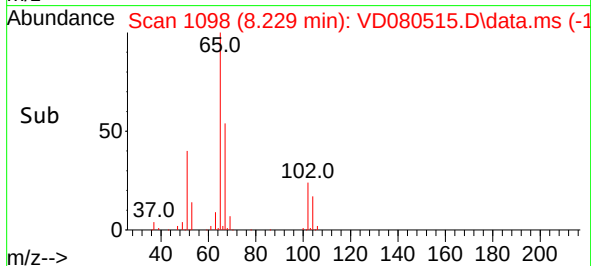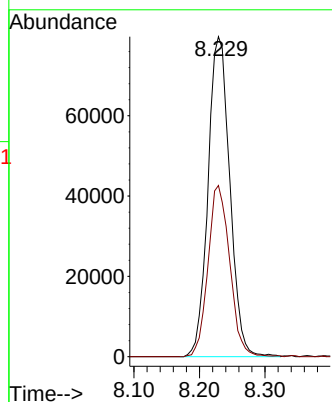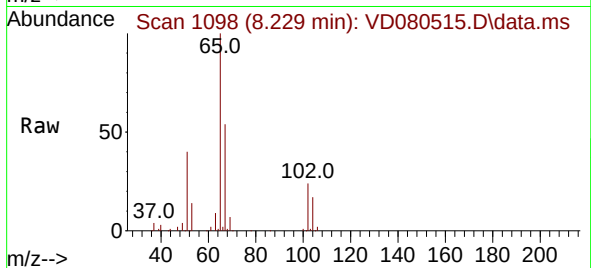

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.776 min Scan# 1191

Delta R.T. -0.000 min

Lab File: VD080515.D

Acq: 05 Sep 2025 09:54




Tgt Ion: 114 Resp: 625107


Ion Ratio Lower Upper

114 100

63 19.9 0.0 38.6

88 15.4 0.0 32.6

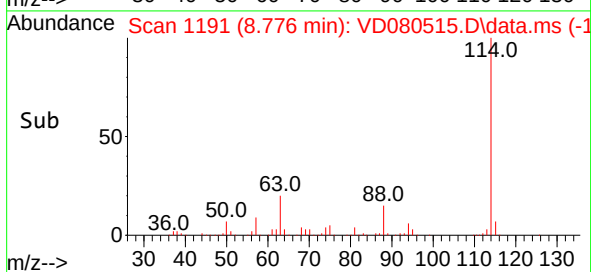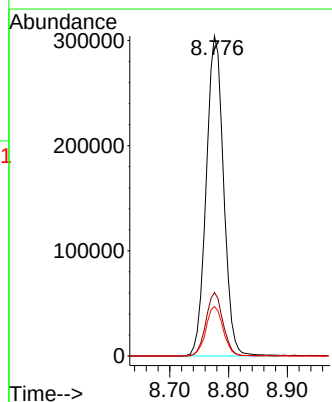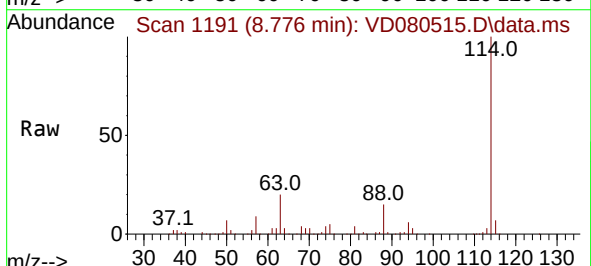

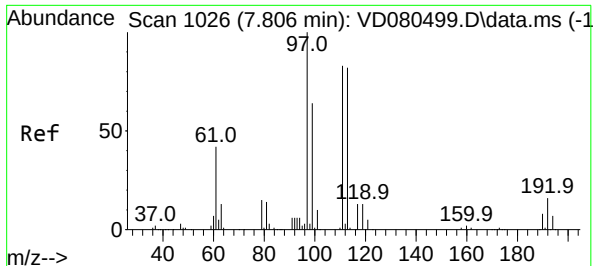

#35

Dibromofluoromethane

Concen: 47.418 ug/l

RT: 7.805 min Scan# 1026

Delta R.T. -0.001 min

Lab File: VD080515.D

Acq: 05 Sep 2025 09:54

Instrument :

MSVOA_D

ClientSampleId :





Tgt Ion:113 Resp: 179913

Ion Ratio Lower Upper

113 100

111 103.6 82.0 123.0

192 18.9 14.9 22.3

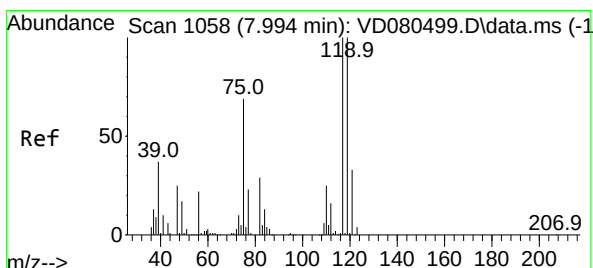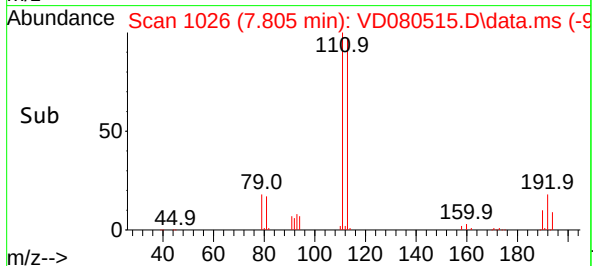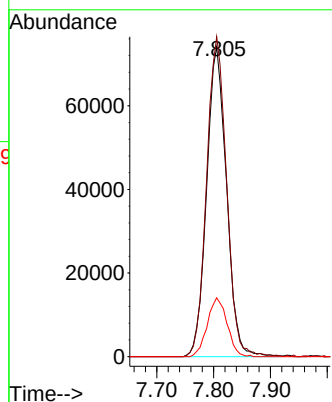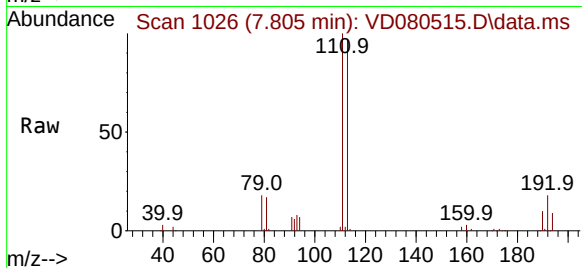

#38

Carbon Tetrachloride

Concen: 6.689 ug/l

RT: 7.876 min Scan# 1038

Delta R.T. -0.118 min

Lab File: VD080515.D

Acq: 05 Sep 2025 09:54




Tgt Ion:117 Resp: 34876


Ion Ratio Lower Upper

117 100

119 3.5 80.2 120.2#

121 0.0 26.8 40.2#


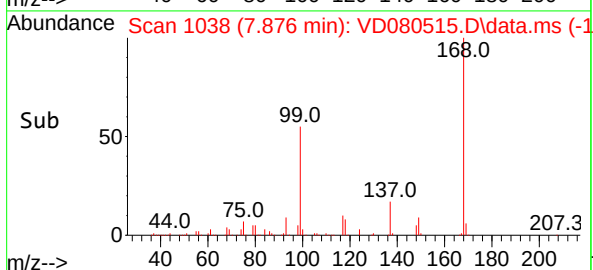
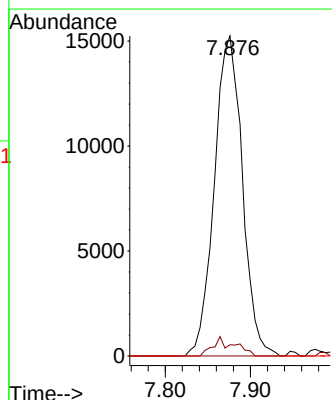
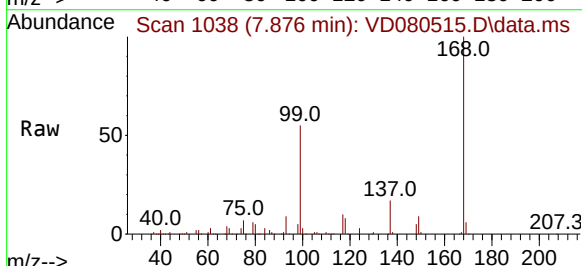


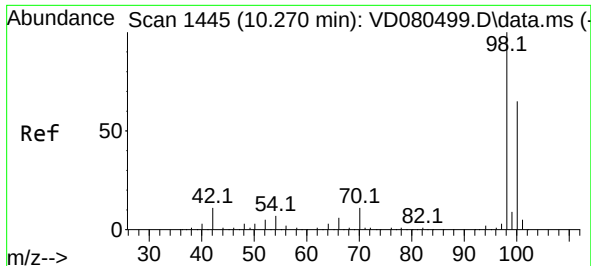

#50
Toluene-d8
Concen: 48.549 ug/l
RT: 10.270 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54




Instrument :
MSVOA_D
ClientSampleId :


Tgt Ion: 98 Resp: 730749
Ion Ratio Lower Upper
98 100
100 65.4 51.8 77.6

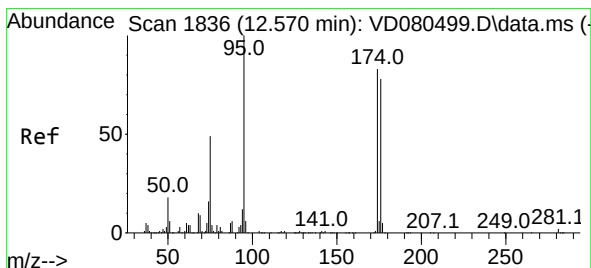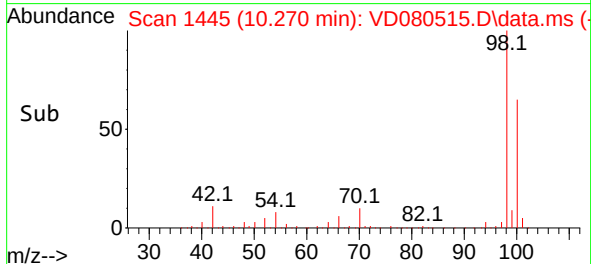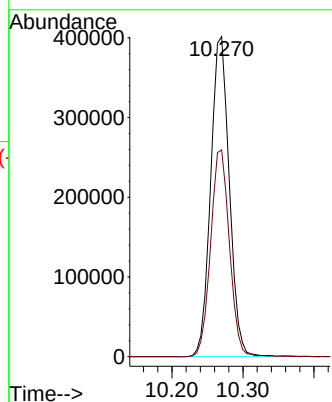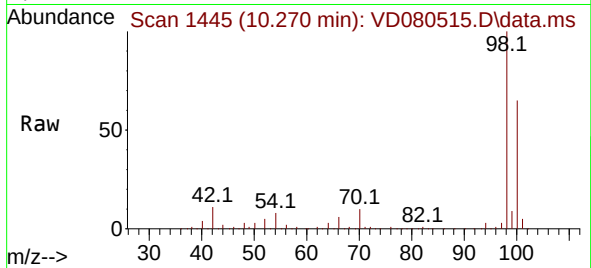

#62
4-Bromofluorobenzene
Concen: 46.781 ug/l
RT: 12.570 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54


Tgt Ion: 95 Resp: 222177
Ion Ratio Lower Upper
95 100
174 83.4 0.0 162.6
176 82.6 0.0 156.0

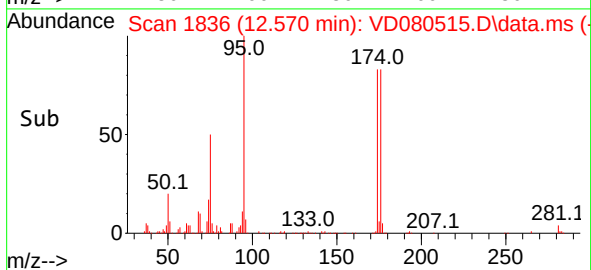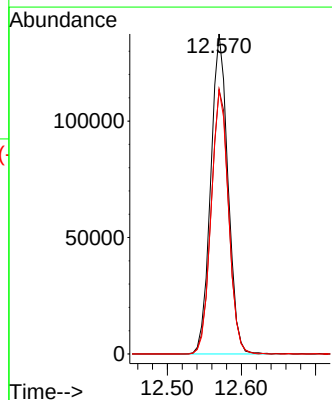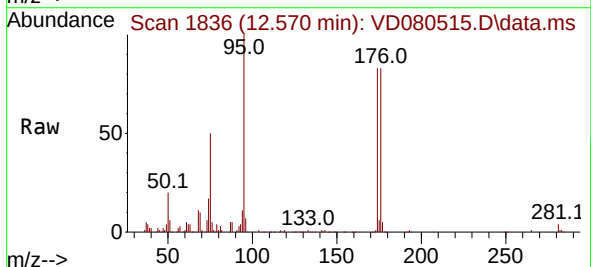



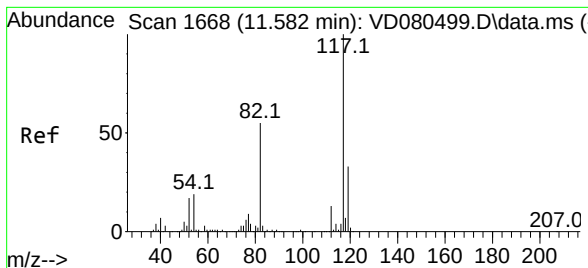


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.582 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54


Instrument :
MSVOA_D
ClientSampleId :

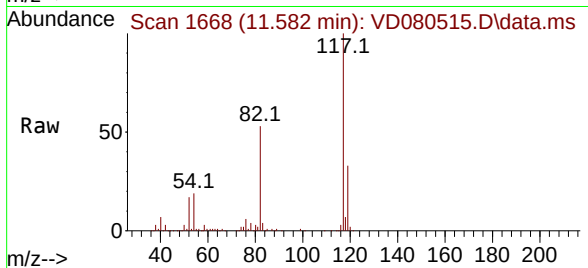



Tgt Ion:117 Resp: 541756
Ion Ratio Lower Upper
117 100
82 53.4 43.8 65.6
119 32.8 26.1 39.1

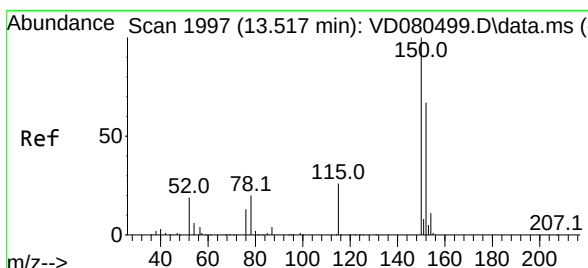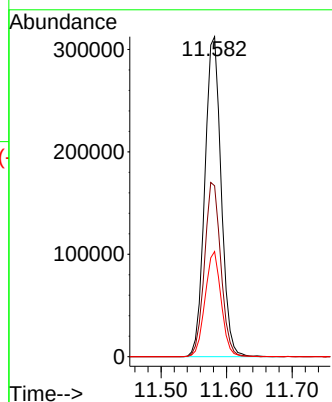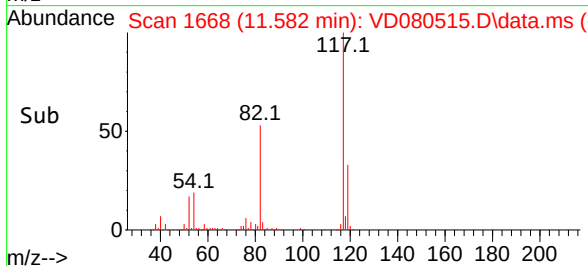


#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.517 min Scan# 1997
Delta R.T. -0.000 min
Lab File: VD080515.D
Acq: 05 Sep 2025 09:54

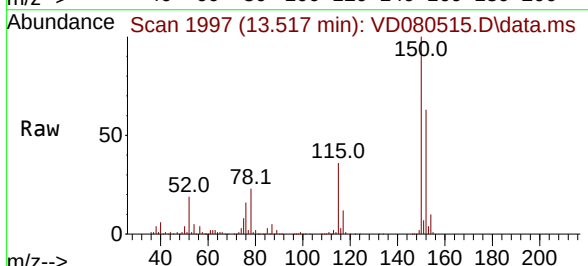

Tgt Ion:152 Resp: 254170
Ion Ratio Lower Upper
152 100
115 58.1 29.0 87.0
150 158.9 0.0 345.0



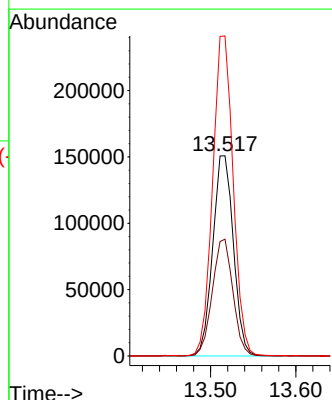
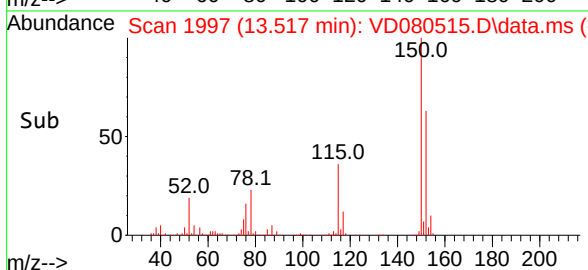


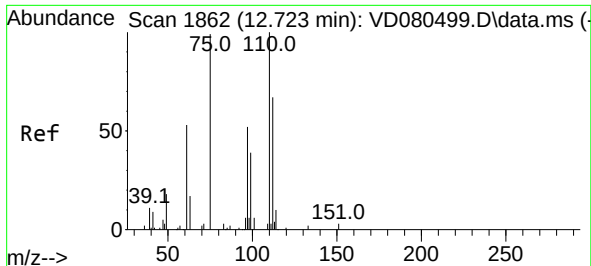

#76
 1,2,3-Trichloropropane
 Concen: 54.540 ug/l
 RT: 12.570 min Scan# 1836
 Delta R.T. -0.153 min
 Lab File: VD080515.D
 Acq: 05 Sep 2025 09:54

Instrument :
 MSVOA_D
 ClientSampleId :

Tgt Ion: 75 Resp: 113138
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

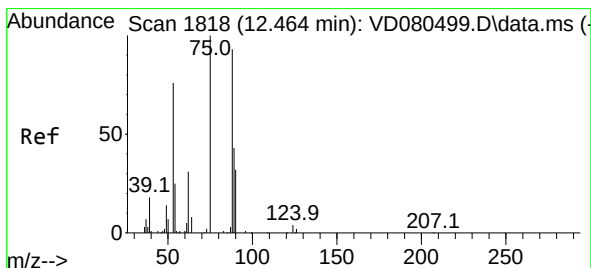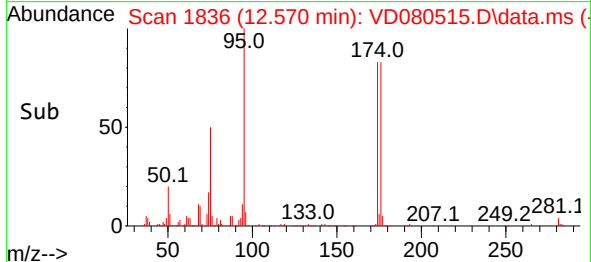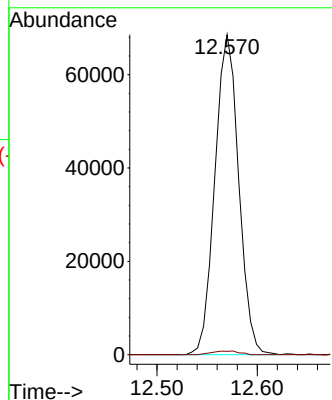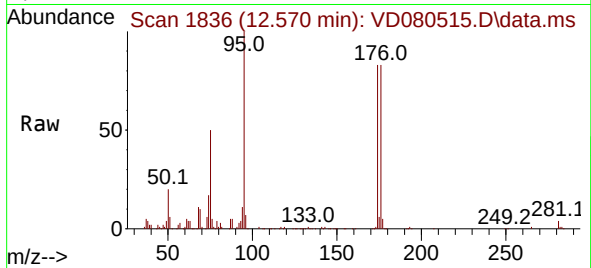

#81
 trans-1,4-Dichloro-2-butene
 Concen: 82.779 ug/l
 RT: 12.570 min Scan# 1836
 Delta R.T. 0.106 min
 Lab File: VD080515.D
 Acq: 05 Sep 2025 09:54

Tgt Ion: 75 Resp: 113138
 Ion Ratio Lower Upper
 75 100
 53 0.0 61.9 92.9#
 89 0.0 34.6 52.0#

