
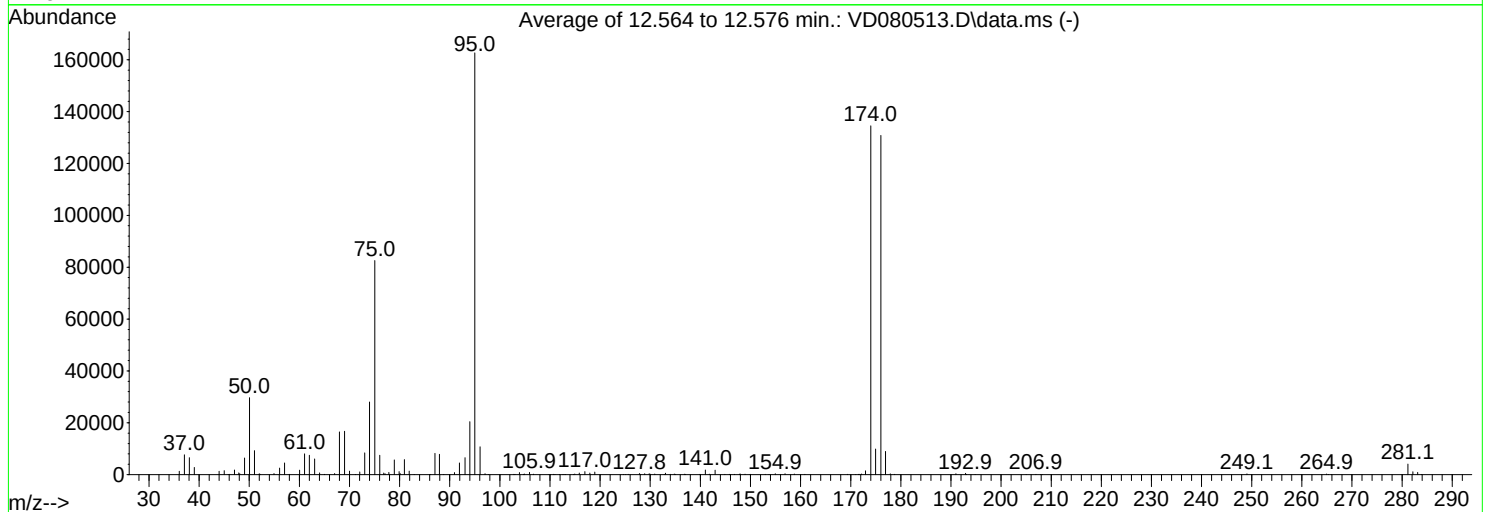


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD080525\
Data File : VD080513.D
Acq On : 05 Sep 2025 08:37
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D082725S.M
Title : SW846 8260
Last Update : Thu Aug 28 03:02:37 2025

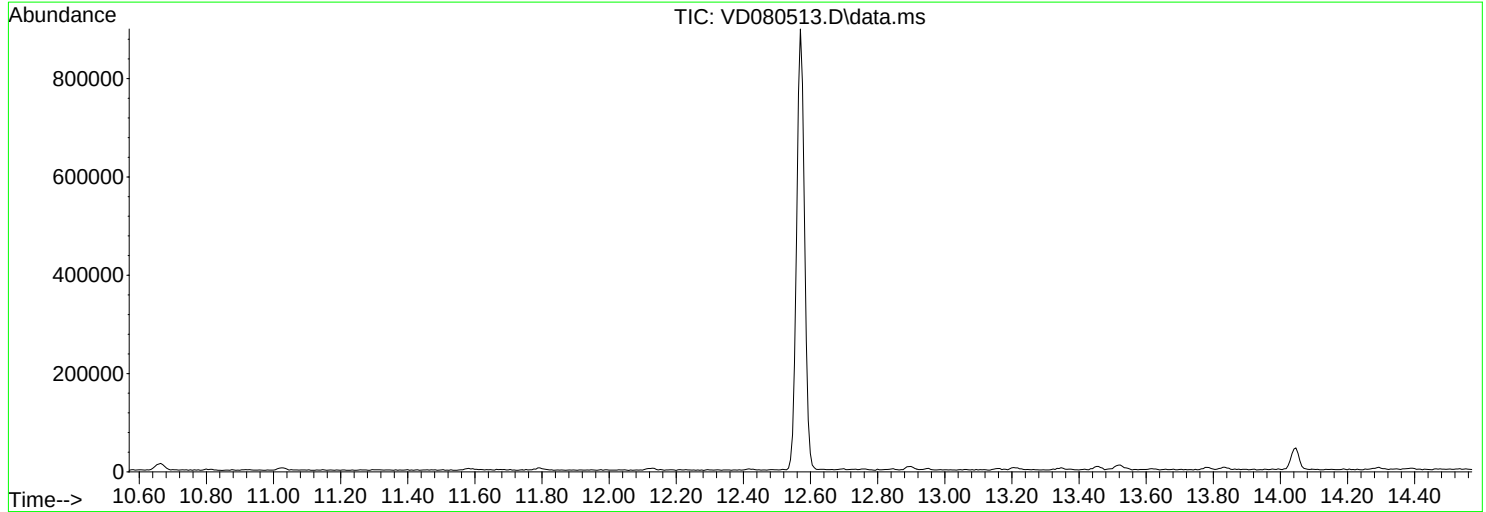

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	29693	PASS
75	95	30	60	50.7	82544	PASS
95	95	100	100	100.0	162688	PASS
96	95	5	9	6.6	10738	PASS
173	174	0.00	2	1.1	1502	PASS
174	95	50	100	82.7	134547	PASS
175	174	5	9	7.4	9892	PASS
176	174	95	101	97.2	130821	PASS
177	176	5	9	6.9	8967	PASS