
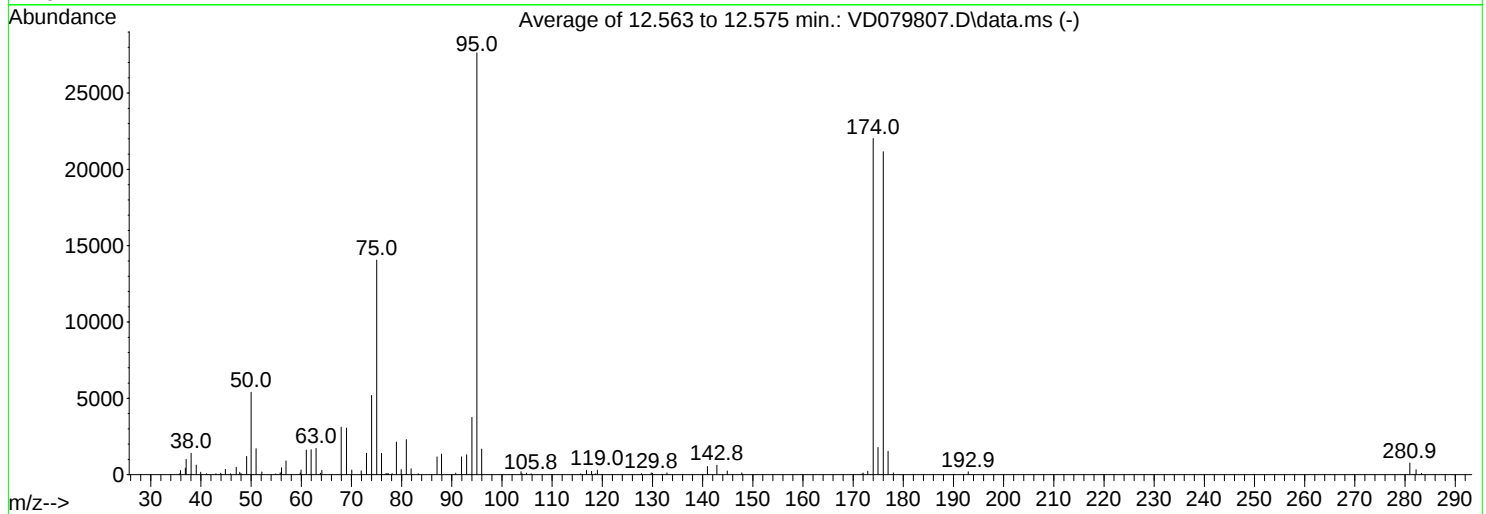


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091024\
Data File : VD079807.D
Acq On : 10 Sep 2024 09:36
Operator : RP/MD
Sample : BFB825
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB825

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Wed Sep 11 06:11:49 2024

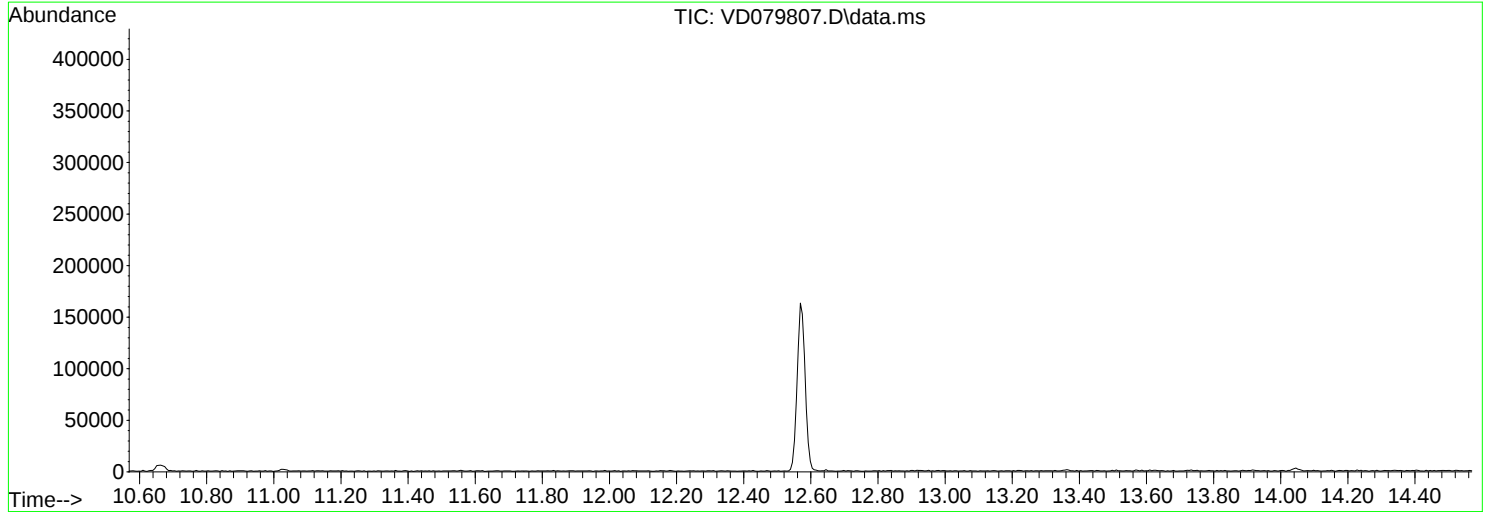

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	5404	PASS
75	95	30	80	50.9	14063	PASS
95	95	100	100	100.0	27635	PASS
96	95	5	9	6.1	1682	PASS
173	174	0.00	2	1.0	223	PASS
174	95	50	120	79.7	22021	PASS
175	174	5	9	8.1	1783	PASS
176	174	95	105	96.1	21160	PASS
177	176	5	10	7.2	1534	PASS

m/z	Abundance
40.00	541.0
44.00	276.0

Instrument :
MSVOA_D
ClientSampleId :
BFB825

m/z	Abundance
35.70	172.0
36.90	1283.0
38.10	1086.0
39.10	573.0
39.90	853.0
43.90	382.0
44.90	373.0
45.90	193.0
47.10	542.0
47.80	270.0
49.10	1314.0
50.00	5009.0
51.00	1302.0
52.20	175.0
56.10	409.0
57.00	700.0
59.80	308.0
61.10	1256.0
62.00	1290.0
63.00	1443.0
63.80	271.0
64.20	215.0
67.90	2833.0
69.00	2224.0
70.10	276.0
71.90	181.0
73.00	873.0
74.00	4467.0
75.00	11493.0
76.00	893.0
76.90	213.0
78.10	191.0
78.90	1635.0
80.90	1829.0
81.90	317.0
87.00	950.0
88.00	1250.0
92.00	957.0
92.90	1361.0
94.00	2799.0
95.00	23984.0
96.00	1337.0
103.80	312.0
105.80	201.0
116.90	173.0
117.90	169.0
119.00	371.0
130.00	271.0
140.90	572.0
142.90	600.0
174.00	17392.0
175.00	1460.0
176.00	18000.0
176.90	1045.0
178.00	191.0
280.90	349.0
282.20	379.0

Instrument :
MSVOA_D
ClientSampleId :
BFB825

m/z	Abundance
35.90	414.0
37.10	1693.0
38.00	1520.0
39.00	690.0
40.00	674.0
43.00	175.0
44.00	318.0
44.80	466.0
47.10	615.0
47.70	193.0
49.10	1179.0
50.00	5317.0
51.00	2014.0
52.20	205.0
54.90	162.0
55.80	385.0
57.00	770.0
60.00	505.0
61.00	2029.0
62.00	2141.0
63.00	1996.0
64.00	311.0
68.00	3279.0
69.00	3765.0
69.90	301.0
72.00	261.0
73.00	1432.0
74.00	5952.0
75.10	16245.0
76.00	1899.0
77.10	262.0
78.90	2422.0
79.90	420.0
81.00	2724.0
81.80	490.0
83.30	181.0
87.10	1555.0
88.00	1347.0
91.90	1330.0
92.90	1399.0
94.00	4355.0
95.00	31904.0
95.90	1619.0
104.00	200.0
105.00	177.0
115.70	164.0
116.80	300.0
117.80	275.0
118.60	185.0
119.00	298.0
129.70	183.0
132.90	154.0
140.90	424.0
142.80	718.0
144.90	333.0
147.80	185.0
171.80	156.0
174.00	25040.0
174.90	1907.0
176.00	23120.0
177.00	1590.0
178.00	165.0
193.10	200.0
280.90	869.0
282.20	189.0

Instrument :
MSVOA_D
ClientSampleId :
BFB825

m/z	Abundance
36.00	413.0
37.00	1316.0
38.10	1622.0
39.10	632.0
40.00	579.0
41.10	178.0
43.90	420.0
44.90	210.0
46.90	277.0
48.00	211.0
49.10	1092.0
50.00	5886.0
51.00	1777.0
52.10	155.0
56.00	930.0
56.90	1244.0
59.90	410.0
60.90	1552.0
61.90	1468.0
62.90	1723.0
64.10	323.0
68.00	3219.0
69.00	3157.0
70.10	333.0
72.00	305.0
73.00	1897.0
74.00	5136.0
75.00	14452.0
76.00	1395.0
77.40	180.0
79.00	2348.0
79.90	583.0
80.90	2321.0
82.00	343.0
87.10	997.0
87.90	1473.0
90.80	329.0
92.00	1215.0
93.00	1150.0
94.00	4118.0
95.00	27016.0
96.00	2089.0
103.80	276.0
104.80	153.0
116.80	368.0
117.80	224.0
119.00	228.0
127.80	176.0
129.80	173.0
132.90	203.0
141.00	617.0
142.90	548.0
144.90	388.0
147.80	156.0
172.00	330.0
172.90	668.0
174.00	23632.0
175.00	1982.0
176.00	22360.0
177.00	1967.0
192.90	353.0
281.00	1084.0
282.20	395.0
283.30	255.0

Instrument :
MSVOA_D
ClientSampleId :
BFB825