
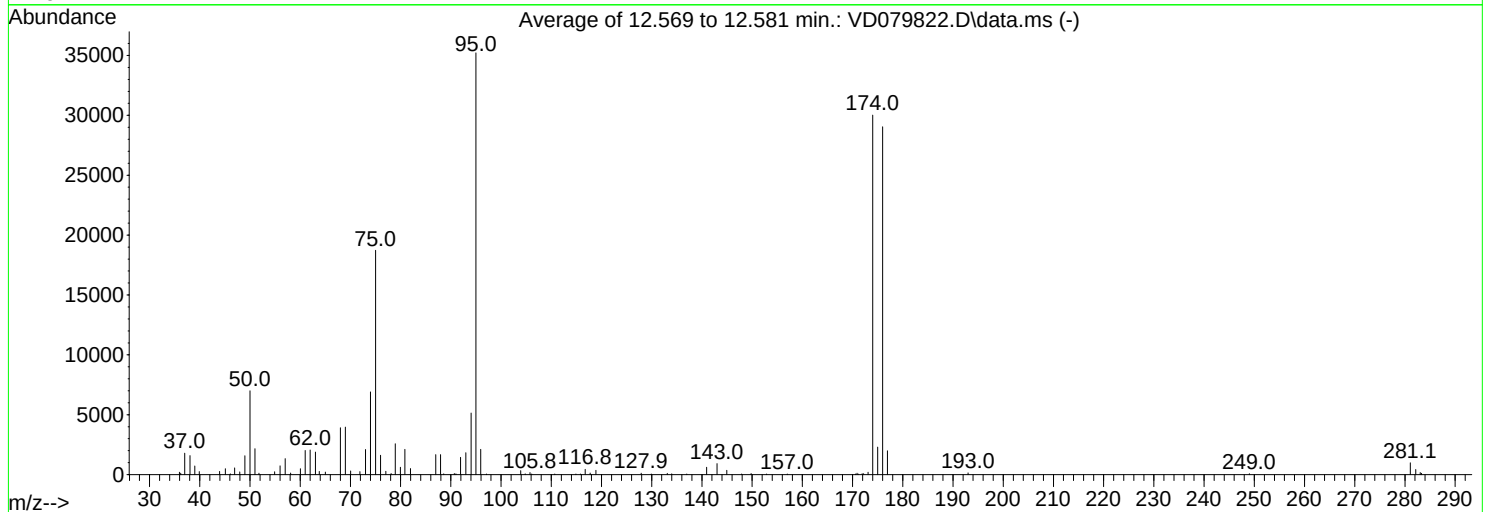


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091224\
Data File : VD079822.D
Acq On : 12 Sep 2024 09:11
Operator : RP/MD
Sample : BFB827
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB827

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Fri Sep 13 23:49:48 2024

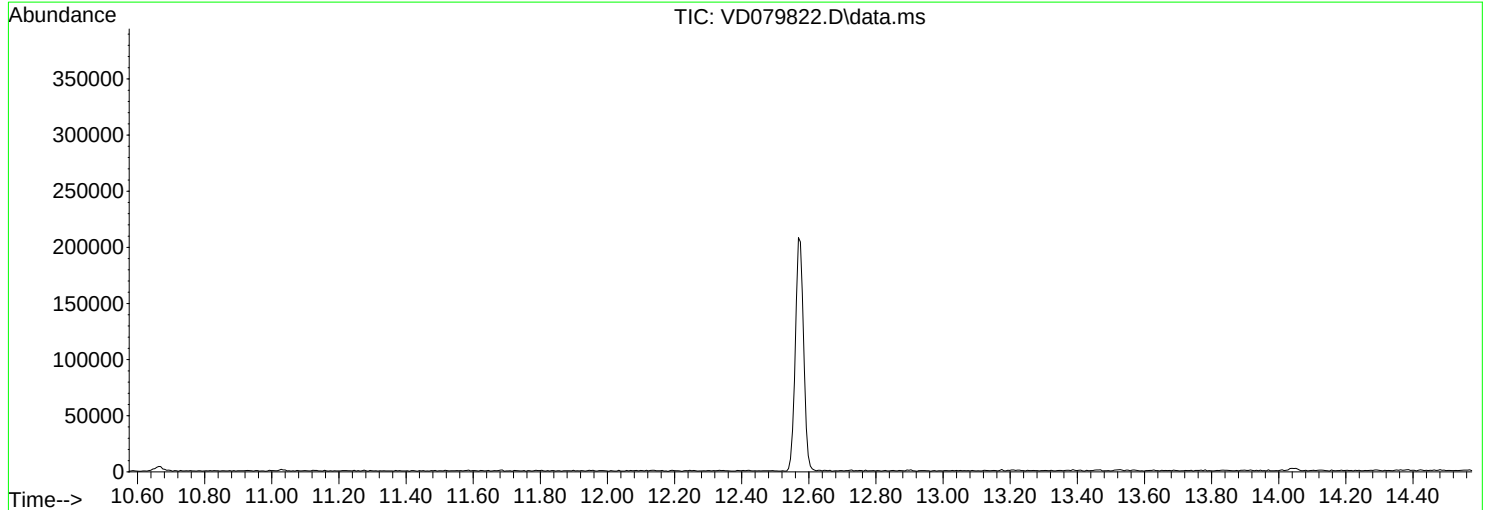

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	7000	PASS
75	95	30	80	53.2	18724	PASS
95	95	100	100	100.0	35216	PASS
96	95	5	9	6.0	2110	PASS
173	174	0.00	2	0.7	205	PASS
174	95	50	120	85.2	30016	PASS
175	174	5	9	7.7	2304	PASS
176	174	95	105	96.8	29045	PASS
177	176	5	10	6.9	1991	PASS

Scan 1860 (12.528 min): VD079822.D\data.ms
BFB827

m/z	Abundance
39.90	507.0
44.00	258.0

Instrument :
MSVOA_D
ClientSampleId :
BFB827

m/z	Abundance
36.20	378.0
37.00	2370.0
38.10	1761.0
39.00	969.0
40.00	834.0
43.90	436.0
45.10	479.0
46.10	199.0
47.00	492.0
48.00	327.0
49.00	1590.0
50.00	7654.0
51.00	2436.0
54.90	251.0
56.10	1036.0
57.00	1270.0
58.10	200.0
60.00	762.0
61.00	2194.0
62.10	2497.0
63.00	2136.0
63.90	290.0
65.00	304.0
68.00	4703.0
69.00	4576.0
70.10	355.0
71.90	465.0
73.00	1965.0
74.00	7417.0
75.00	20192.0
76.00	1802.0
77.20	311.0
78.10	287.0
79.00	2822.0
80.00	574.0
80.80	2267.0
81.90	410.0
87.00	2231.0
88.00	1880.0
91.00	214.0
91.90	1288.0
93.00	2182.0
94.00	5986.0
95.00	37416.0
96.00	2370.0
104.00	404.0
105.80	334.0
116.80	708.0
117.80	237.0
119.00	398.0
128.00	182.0
129.90	151.0
141.10	555.0
142.90	1217.0
144.90	496.0
147.90	157.0
149.80	268.0
157.00	155.0
170.90	351.0
173.10	616.0
174.00	32144.0
175.00	2589.0
176.00	31528.0
177.00	2146.0
281.00	1022.0
282.10	277.0
283.10	202.0

Instrument :
MSVOA_D
ClientSampleId :
BFB827

m/z	Abundance
35.90	355.0
37.00	1658.0
38.10	1730.0
39.00	806.0
40.00	783.0
44.00	592.0
45.10	454.0
47.00	758.0
47.90	372.0
49.00	1659.0
50.00	7323.0
51.00	2472.0
51.90	209.0
54.90	319.0
55.90	730.0
57.00	1582.0
58.10	212.0
60.10	477.0
61.00	2126.0
61.90	1979.0
63.10	1901.0
63.80	340.0
65.00	169.0
68.00	4076.0
69.00	4111.0
70.00	363.0
71.90	283.0
73.00	2496.0
74.00	7460.0
75.00	20752.0
76.00	1585.0
77.00	522.0
78.90	2808.0
80.00	538.0
80.90	2450.0
81.90	455.0
87.00	1695.0
87.90	1862.0
90.70	279.0
91.90	1760.0
93.00	1710.0
94.10	5450.0
95.00	38320.0
95.90	2033.0
97.10	171.0
103.80	381.0
106.10	163.0
110.70	167.0
115.80	150.0
116.70	291.0
117.70	175.0
118.80	448.0
127.80	197.0
133.20	167.0
134.00	185.0
137.00	154.0
140.90	690.0
143.00	958.0
145.00	287.0
170.60	163.0
171.10	175.0
172.20	226.0
174.00	32408.0
175.00	2103.0
176.00	31128.0
176.90	2141.0
193.00	155.0
281.00	850.0
282.10	514.0
283.30	307.0

Instrument :
MSVOA_D
ClientSampleId :
BFB827

m/z	Abundance
36.00	258.0
37.00	1337.0
38.00	1286.0
39.10	412.0
39.90	649.0
43.90	540.0
45.10	549.0
46.80	440.0
49.00	1501.0
50.00	6022.0
51.00	1602.0
51.70	164.0
54.90	170.0
56.00	446.0
57.00	1142.0
59.90	234.0
61.00	1725.0
62.00	1687.0
63.10	1598.0
63.70	195.0
65.10	156.0
68.00	2983.0
69.00	3204.0
70.00	218.0
73.00	1831.0
74.00	5829.0
75.00	15227.0
76.00	1473.0
78.90	2118.0
79.90	719.0
80.90	1629.0
82.00	642.0
87.00	1102.0
87.90	1275.0
88.60	217.0
92.00	1300.0
93.00	1586.0
94.00	4009.0
95.00	29912.0
96.00	1928.0
103.90	234.0
104.80	185.0
105.70	200.0
114.90	155.0
116.80	333.0
118.90	250.0
133.00	154.0
140.80	588.0
143.10	581.0
144.90	301.0
152.90	155.0
171.90	245.0
174.00	25496.0
175.00	2219.0
176.00	24480.0
177.00	1687.0
193.00	311.0
249.00	238.0
281.10	1103.0
282.20	505.0
283.00	310.0

Instrument :
MSVOA_D
ClientSampleId :
BFB827