
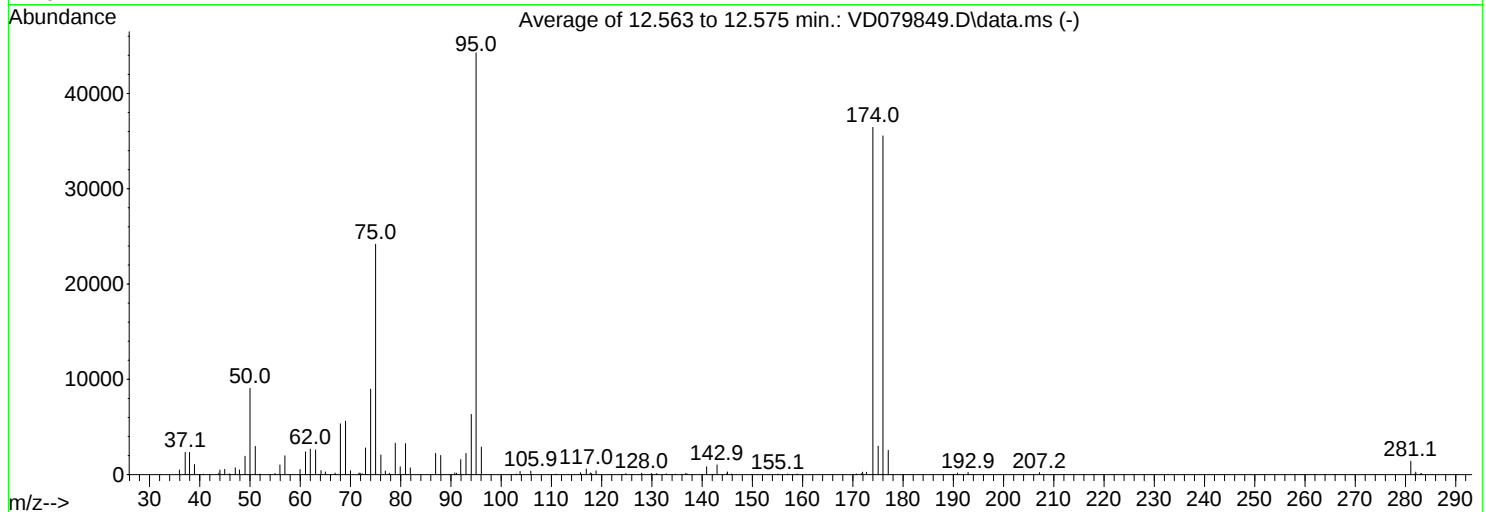


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD091724\
Data File : VD079849.D
Acq On : 17 Sep 2024 09:19
Operator : RP/MD
Sample : BFB830
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB830

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Wed Sep 18 04:50:50 2024

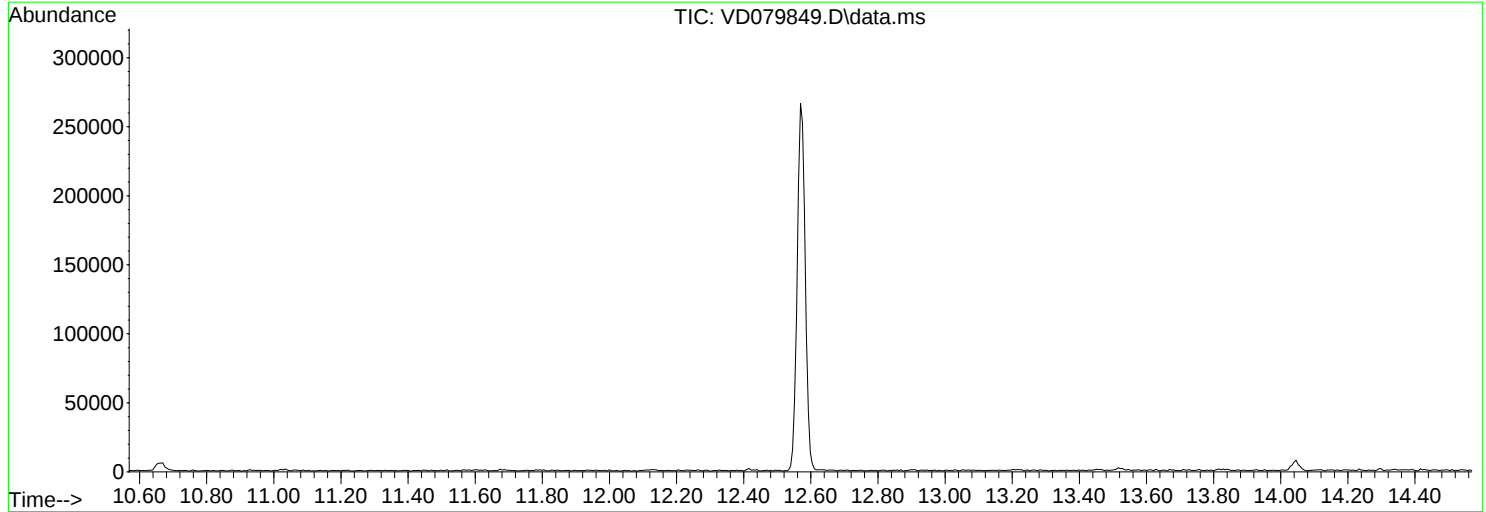

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	9075	PASS
75	95	30	80	54.6	24179	PASS
95	95	100	100	100.0	44261	PASS
96	95	5	9	6.5	2887	PASS
173	174	0.00	2	0.7	244	PASS
174	95	50	120	82.4	36459	PASS
175	174	5	9	8.2	2990	PASS
176	174	95	105	97.5	35539	PASS
177	176	5	10	7.2	2555	PASS

m/z	Abundance
40.00	907.0

Instrument :
MSVOA_D
ClientSampleId :
BFB830

m/z	Abundance
35.90	329.0
37.10	2086.0
37.90	2216.0
38.90	1096.0
40.10	528.0
43.80	435.0
44.90	564.0
45.90	289.0
47.00	616.0
47.80	286.0
49.00	1960.0
50.00	7546.0
51.00	2892.0
55.00	172.0
55.90	977.0
56.90	1520.0
59.90	426.0
61.00	2072.0
62.00	2240.0
63.10	2273.0
64.10	447.0
64.90	154.0
68.00	4691.0
69.00	4258.0
69.90	400.0
71.70	300.0
72.90	2337.0
74.00	7579.0
75.00	20800.0
76.10	1530.0
76.90	333.0
78.90	3167.0
79.90	893.0
80.90	2982.0
82.00	739.0
87.00	1843.0
87.90	1924.0
91.10	198.0
92.00	1555.0
93.00	1649.0
94.00	5766.0
95.00	38704.0
96.00	2543.0
103.70	274.0
105.90	243.0
116.90	537.0
117.70	268.0
118.90	398.0
127.90	251.0
129.80	159.0
136.80	203.0
140.80	741.0
142.20	152.0
143.00	810.0
144.90	326.0
155.10	224.0
170.70	269.0
172.00	335.0
174.00	31944.0
175.10	2470.0
176.00	29392.0
177.00	2281.0
193.00	178.0
207.10	280.0
281.00	1141.0
281.80	219.0

Instrument :
MSVOA_D
ClientSampleId :
BFB830

m/z	Abundance
36.00	415.0
37.10	2662.0
38.00	2469.0
39.00	1173.0
39.90	630.0
44.00	877.0
45.00	611.0
47.10	927.0
47.90	767.0
49.00	2122.0
50.00	9893.0
51.00	3142.0
52.00	199.0
55.00	241.0
56.00	1106.0
57.00	2331.0
59.90	533.0
61.00	2867.0
62.00	2795.0
63.00	2623.0
64.10	506.0
65.00	262.0
67.00	346.0
68.00	5431.0
69.00	6781.0
70.00	341.0
71.90	526.0
73.00	3355.0
74.00	10174.0
75.00	26392.0
75.90	2107.0
76.80	213.0
77.80	256.0
78.90	3832.0
79.80	728.0
80.90	3090.0
82.00	467.0
86.90	2763.0
87.90	2168.0
90.80	326.0
91.90	1591.0
93.00	2060.0
94.10	6293.0
95.00	48424.0
96.00	3110.0
103.00	192.0
103.80	349.0
105.90	504.0
115.80	216.0
117.00	545.0
117.80	311.0
118.90	397.0
124.80	181.0
130.00	153.0
131.00	154.0
132.90	237.0
134.70	161.0
136.70	211.0
140.90	922.0
143.00	1040.0
145.10	587.0
145.80	213.0
158.90	196.0
171.70	364.0
174.00	39792.0
175.00	3050.0
176.00	41136.0
177.00	3046.0
190.90	270.0
192.80	272.0
207.20	365.0
281.10	1531.0
282.10	389.0
283.00	244.0

Instrument :
MSVOA_D
ClientSampleId :
BFB830

m/z	Abundance
36.00	734.0
37.10	2260.0
38.00	2300.0
39.00	904.0
40.00	792.0
40.70	167.0
44.00	604.0
44.90	479.0
47.00	641.0
48.00	478.0
49.00	1694.0
50.00	9786.0
51.10	2884.0
55.90	922.0
56.90	2070.0
60.00	675.0
61.10	2225.0
62.00	3026.0
63.00	2910.0
64.20	349.0
65.00	435.0
66.90	167.0
68.00	5909.0
69.00	5773.0
70.10	474.0
71.70	190.0
72.30	310.0
73.10	2707.0
74.00	9139.0
75.00	25344.0
76.10	2588.0
77.00	576.0
77.70	220.0
78.90	2944.0
80.00	862.0
81.00	3693.0
81.80	891.0
86.90	2104.0
88.00	1950.0
90.70	223.0
91.10	245.0
92.00	1595.0
93.00	2994.0
94.10	6918.0
95.00	45656.0
96.10	3007.0
103.80	402.0
105.90	395.0
110.90	201.0
115.80	377.0
116.90	666.0
118.00	377.0
118.90	431.0
124.80	184.0
128.00	186.0
129.90	204.0
130.90	178.0
137.00	250.0
141.00	788.0
142.90	1218.0
145.00	251.0
157.00	226.0
171.90	475.0
172.70	731.0
174.00	37640.0
175.00	3450.0
176.00	36088.0
177.10	2338.0
190.80	220.0
193.00	240.0
281.00	1579.0
282.00	431.0
283.20	346.0

Instrument :
MSVOA_D
ClientSampleId :
BFB830