



Chlorodifluoromethane

Response Ratio

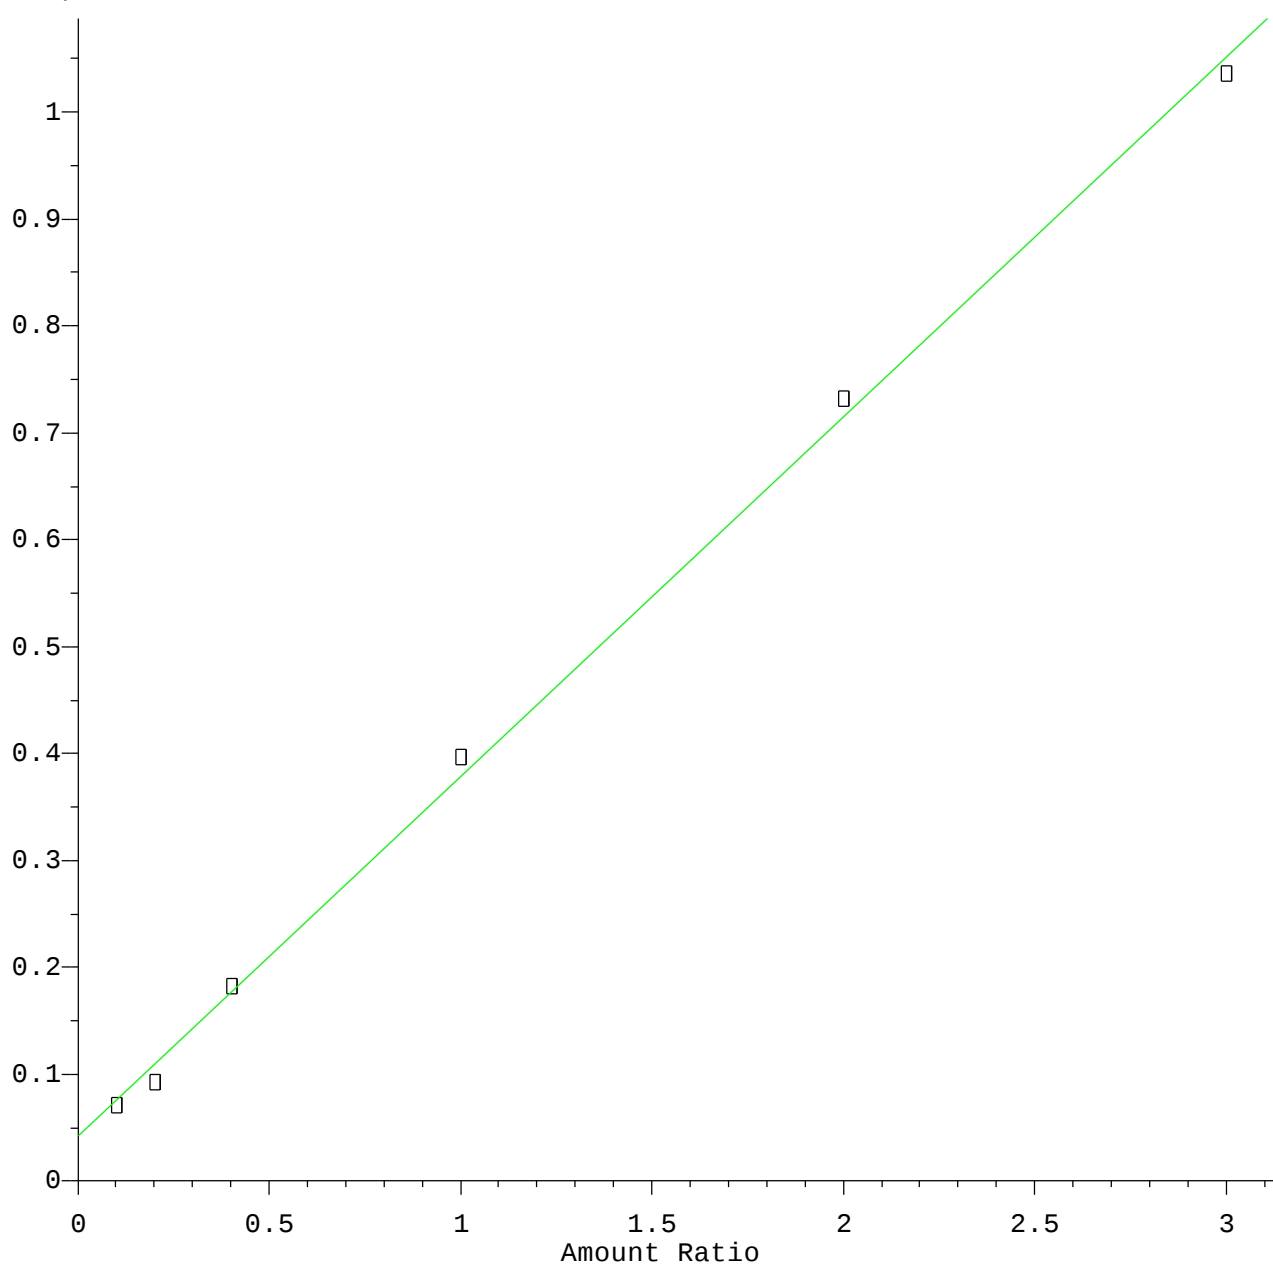


Resp Ratio = $3.36 \times 10^{-1} \times \text{Amt} + 4.23 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

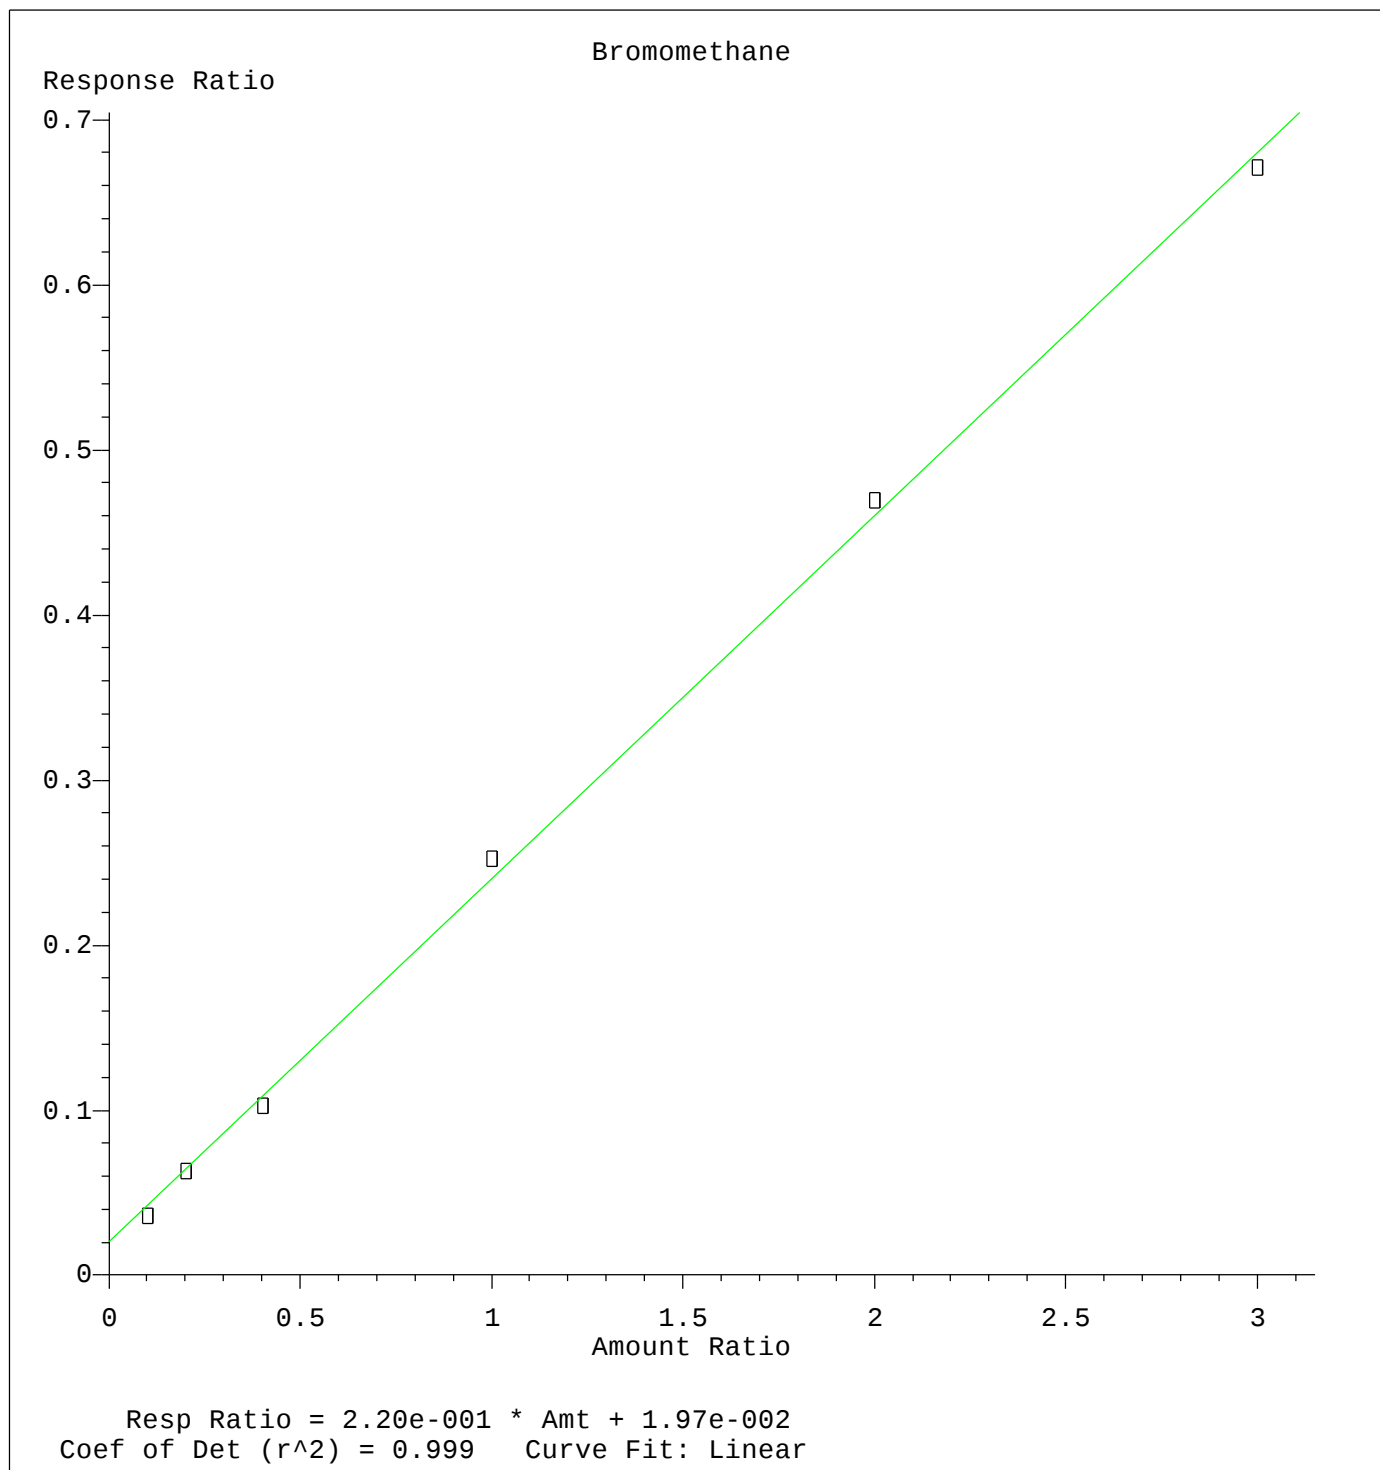


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

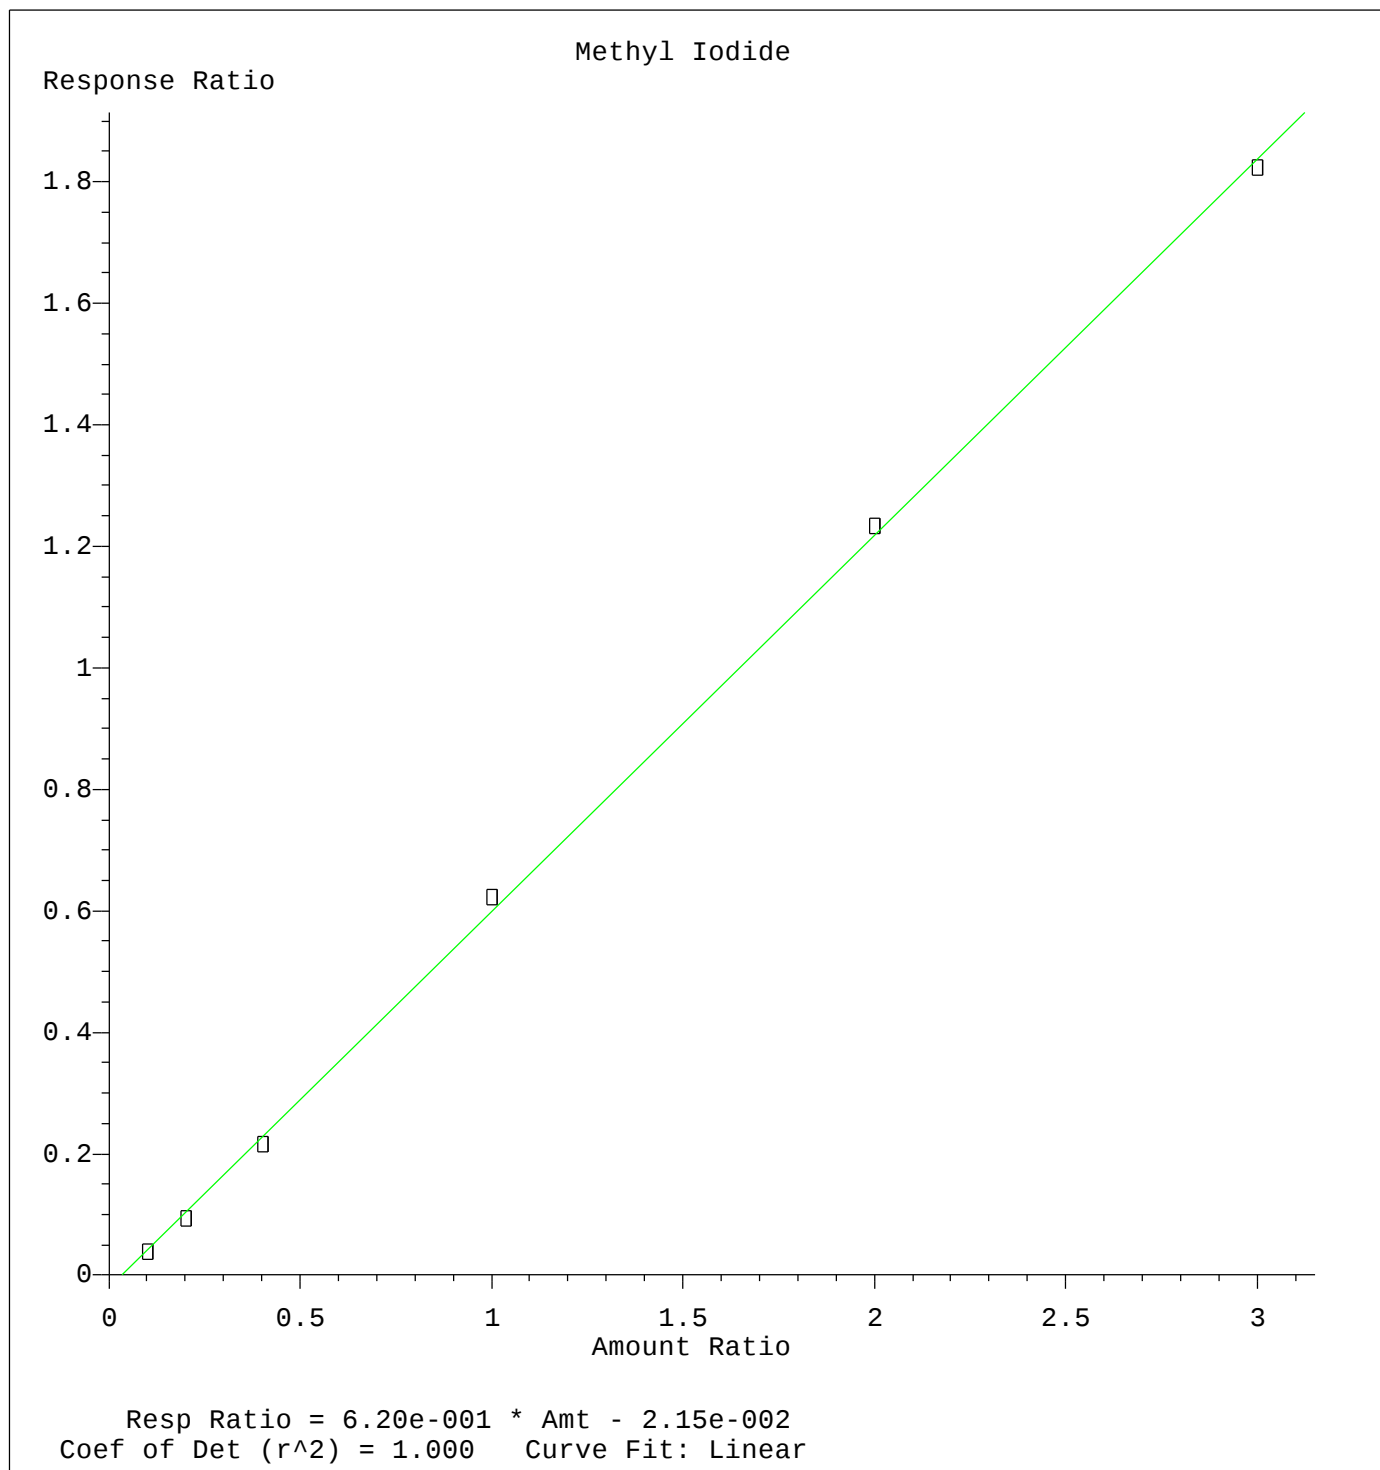


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

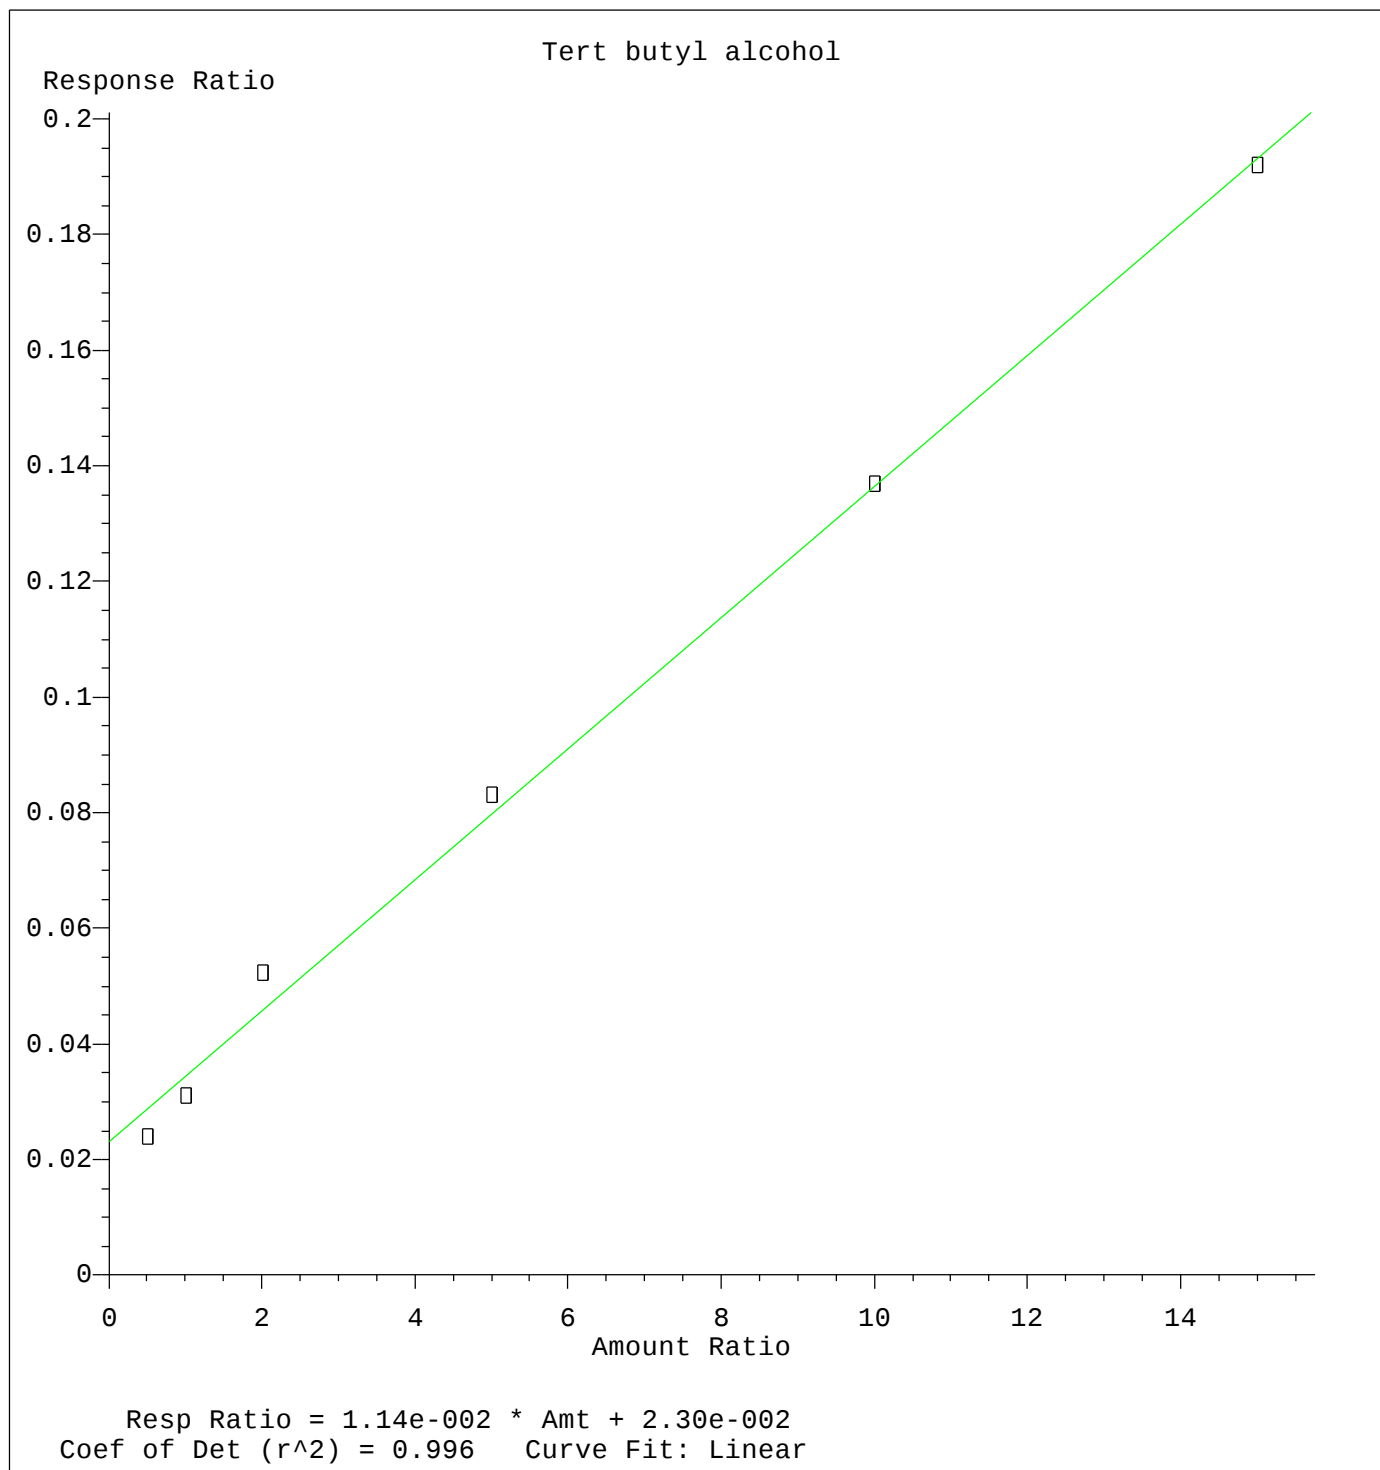

Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

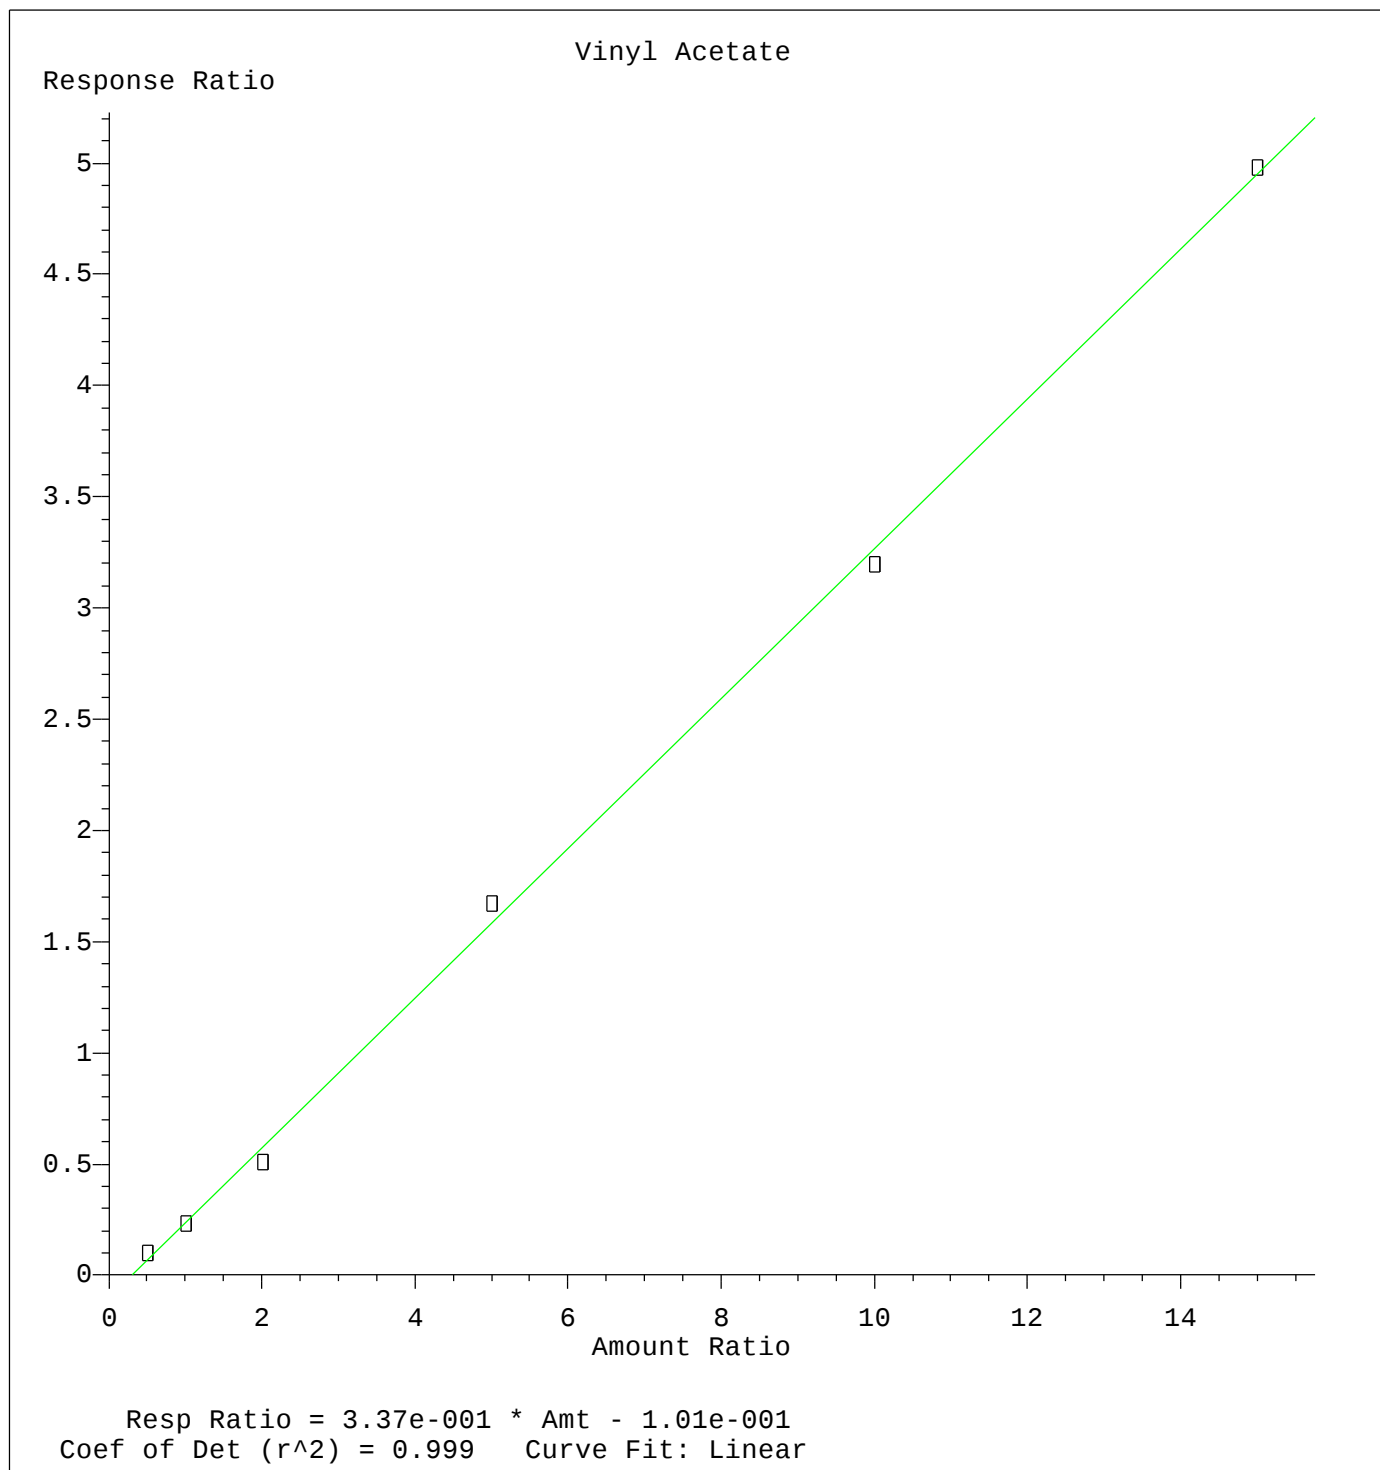


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

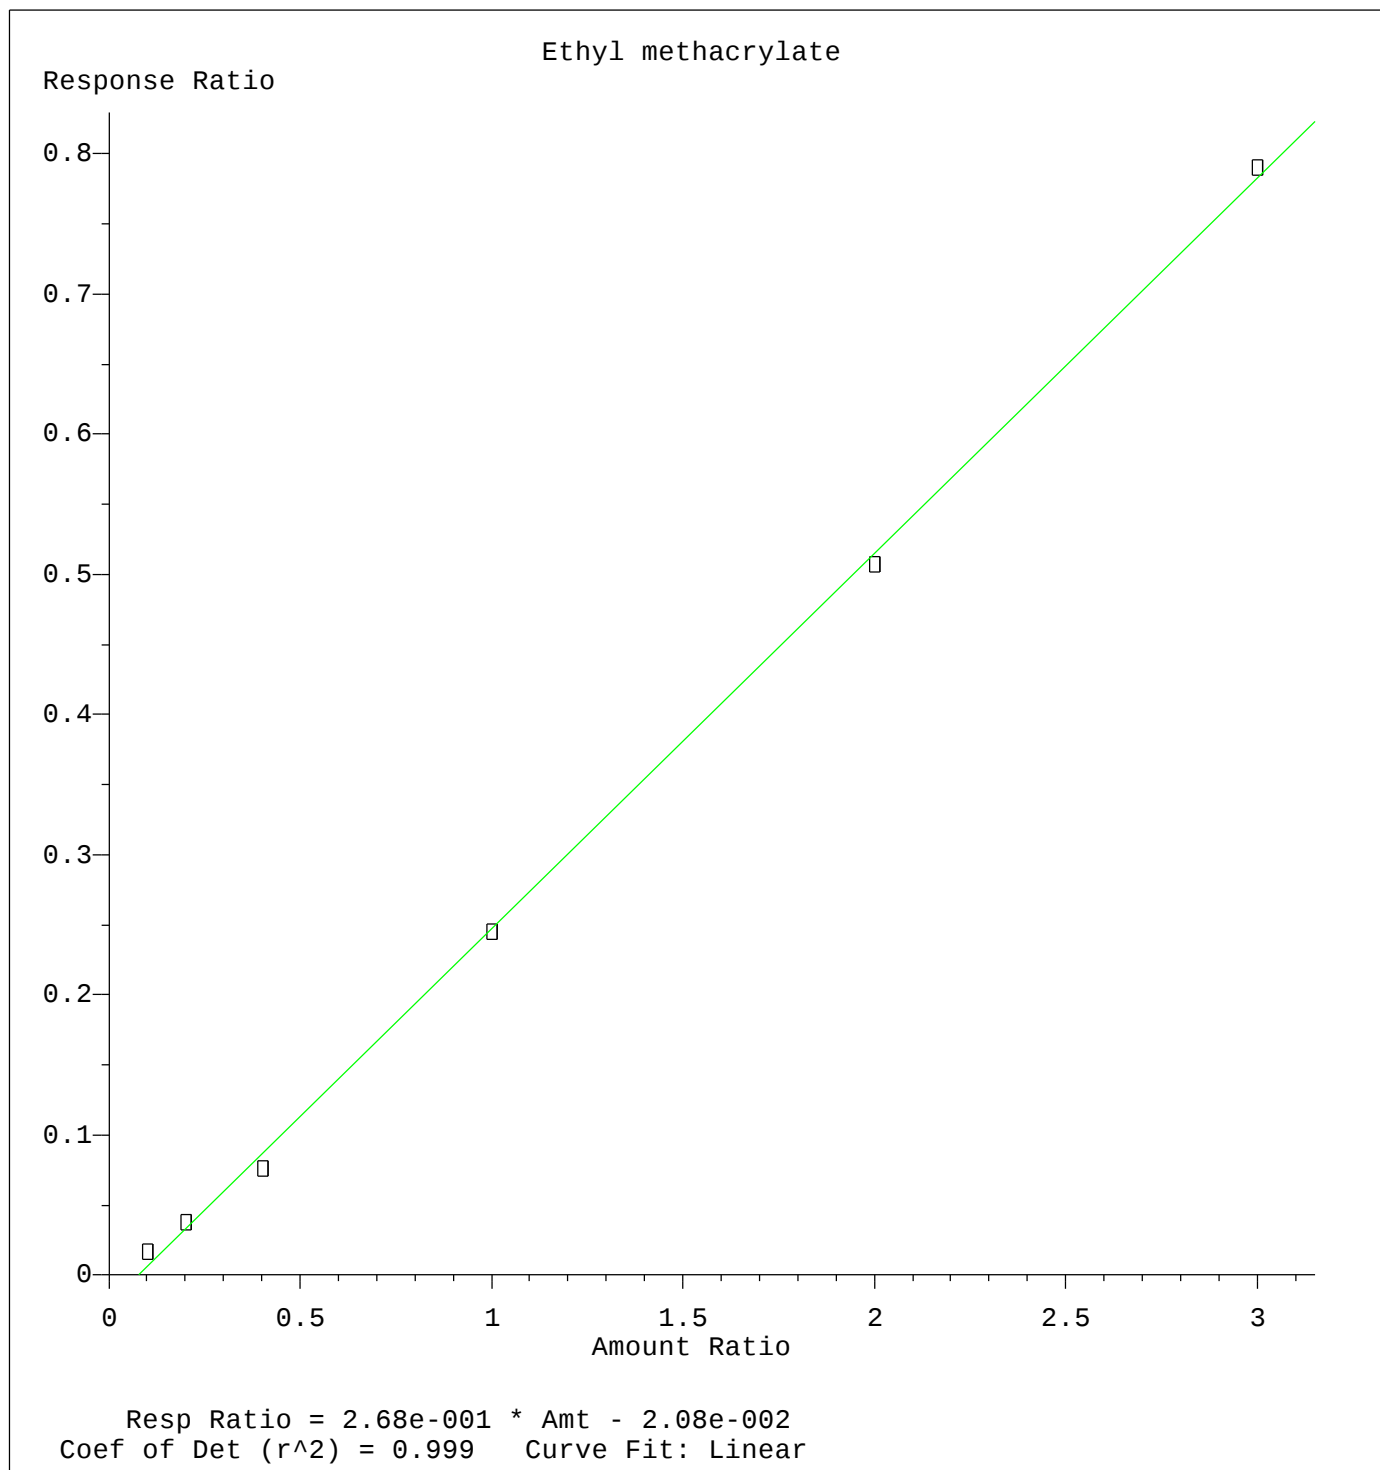

Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015


2-Chloroethyl Vinyl ether

Response Ratio

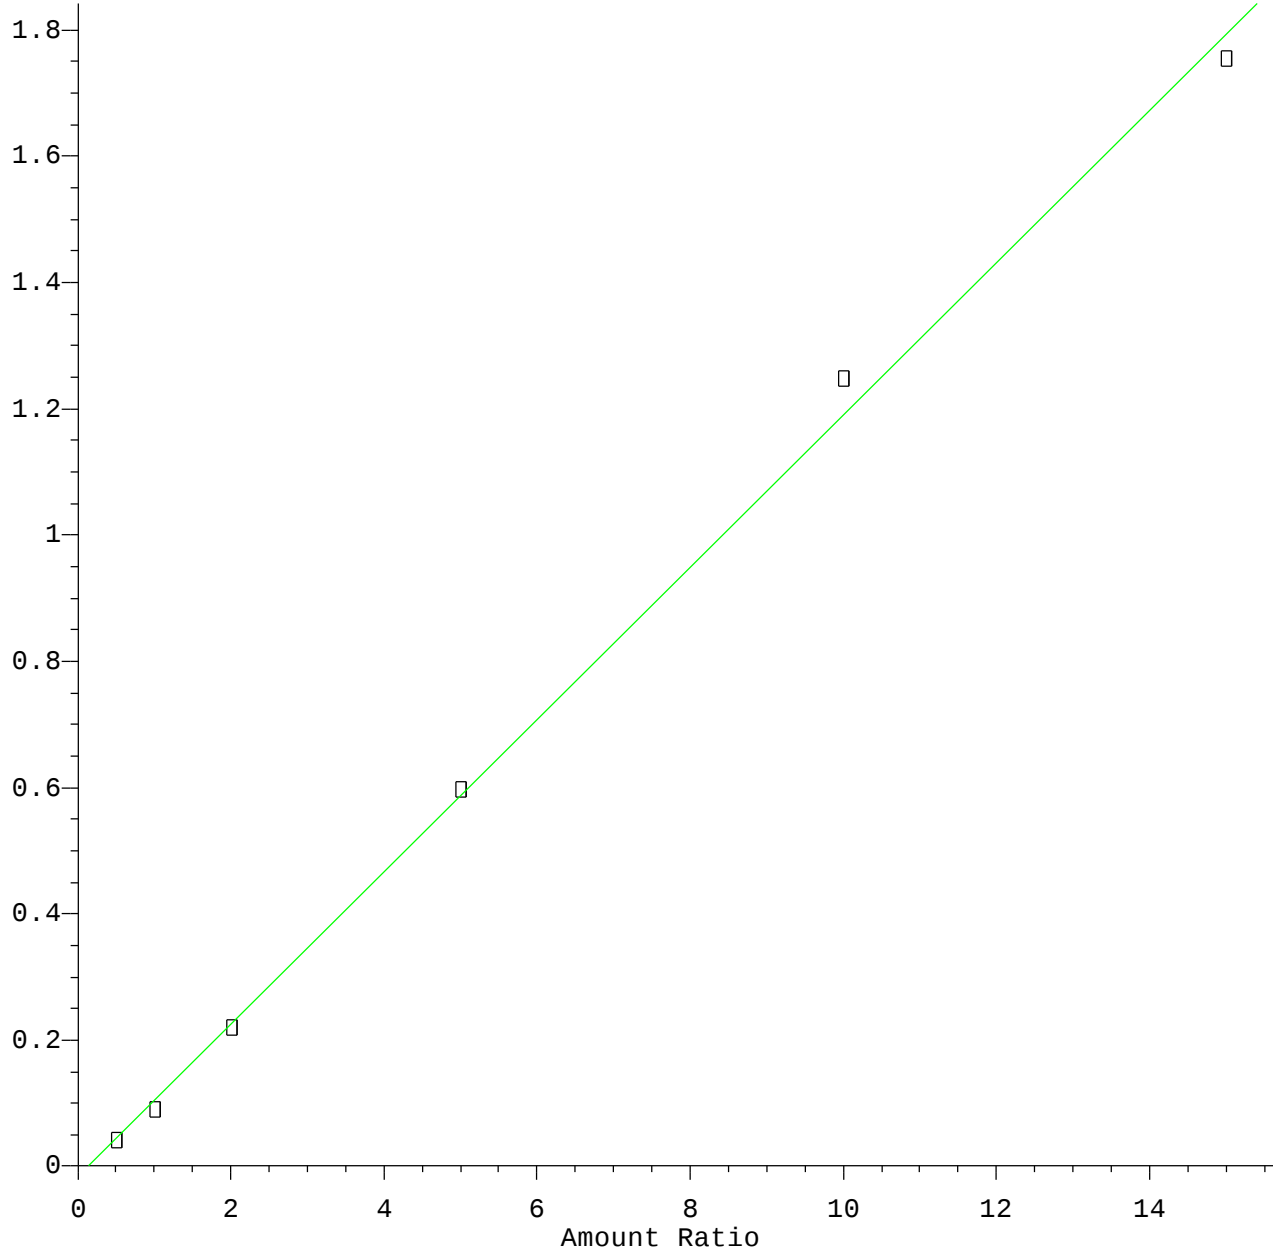


Resp Ratio = $1.21 \times 10^{-1} \times \text{Amt} - 1.53 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

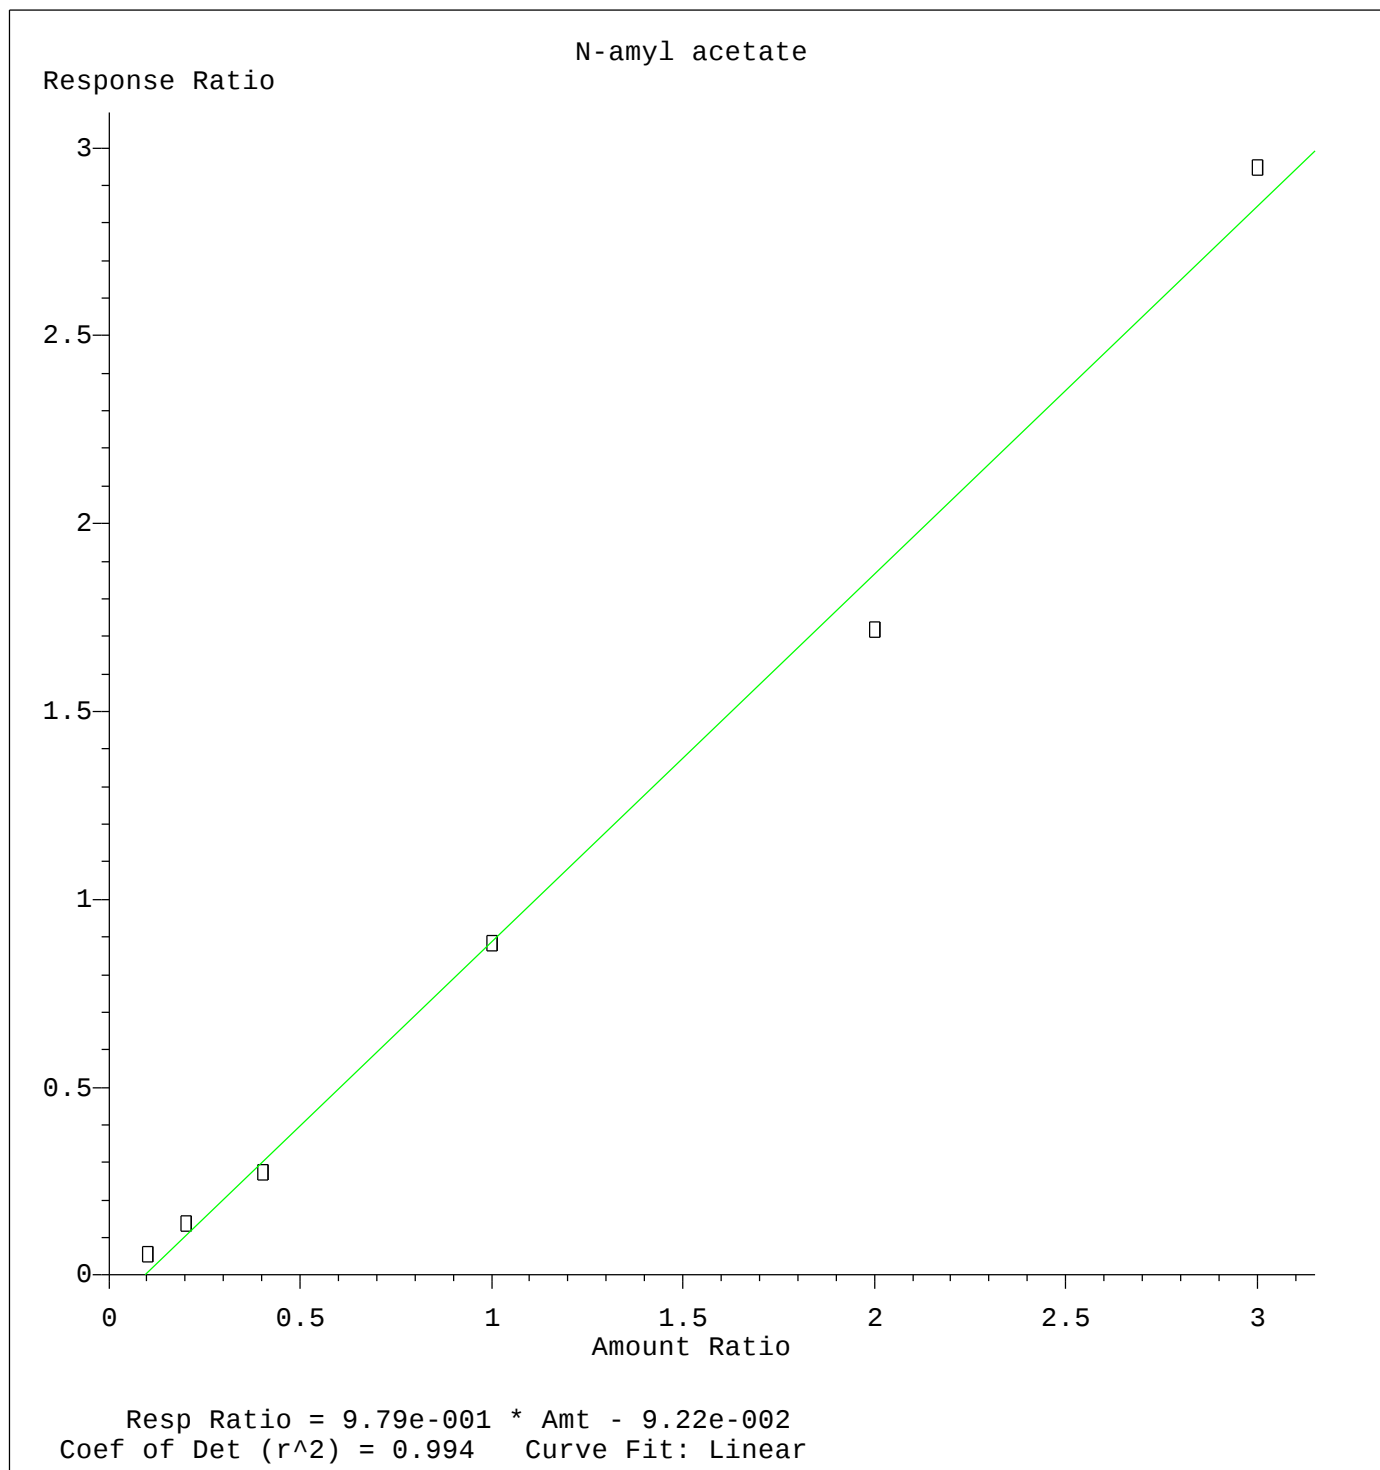


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

trans-1,4-Dichloro-2-butene

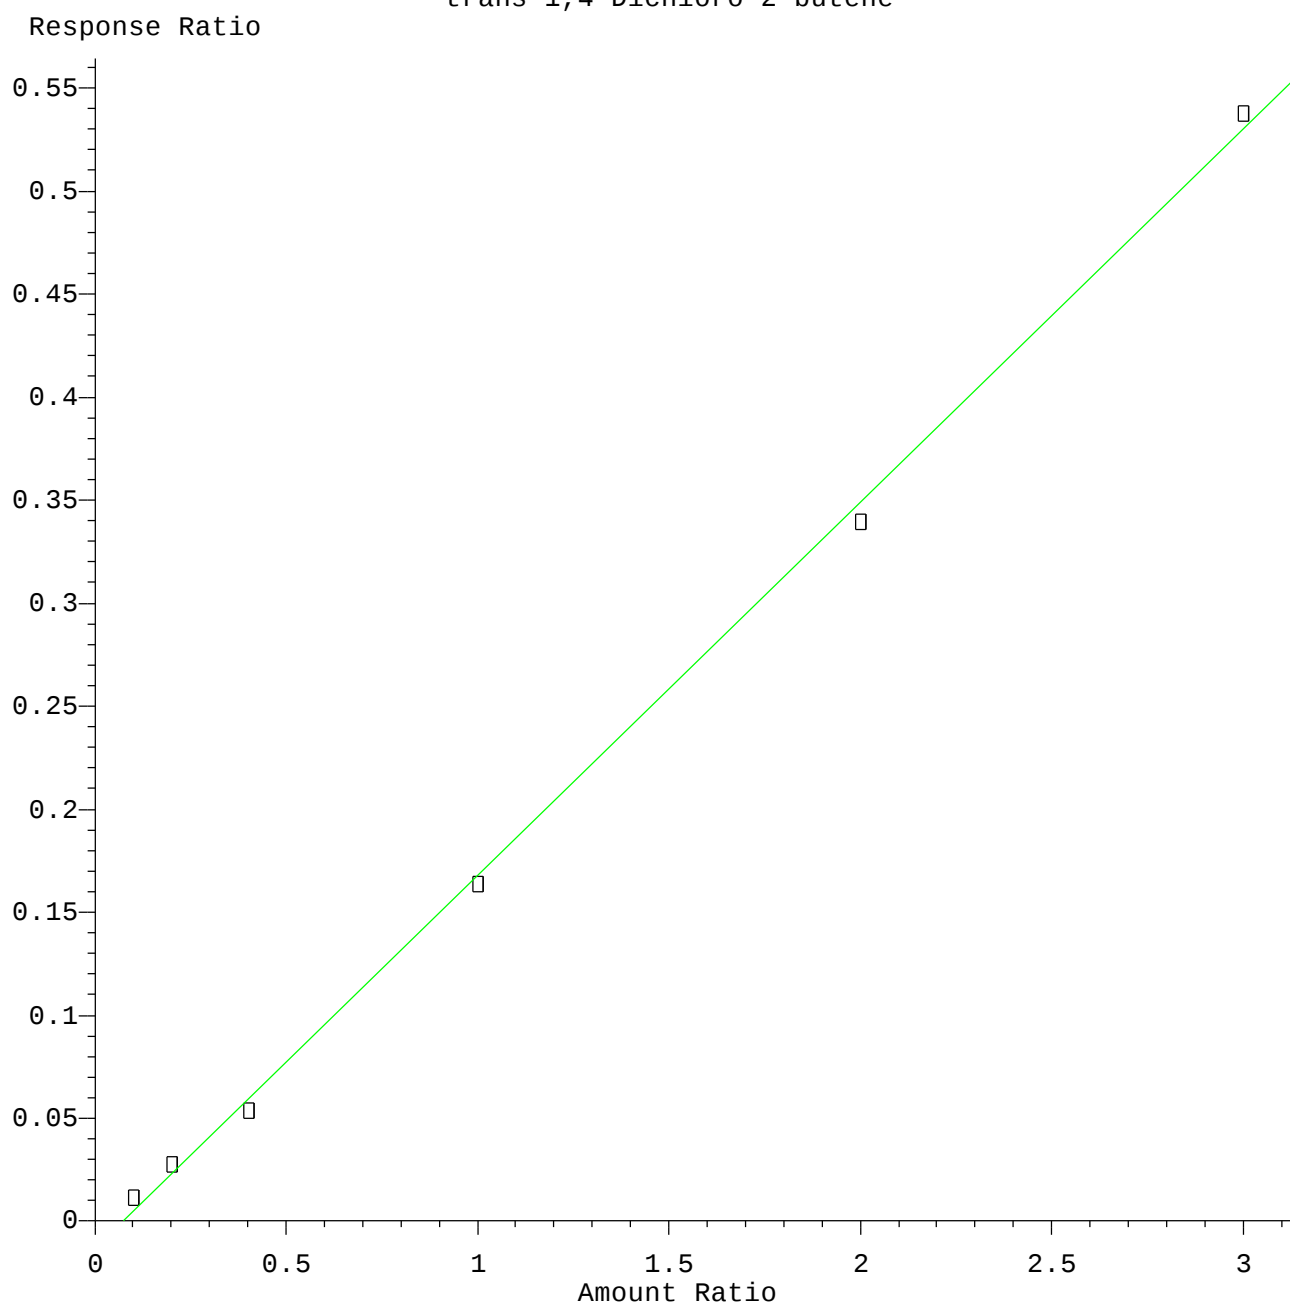

Resp Ratio = $1.81 \times 10^{-1} \times \text{Amt} - 1.36 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

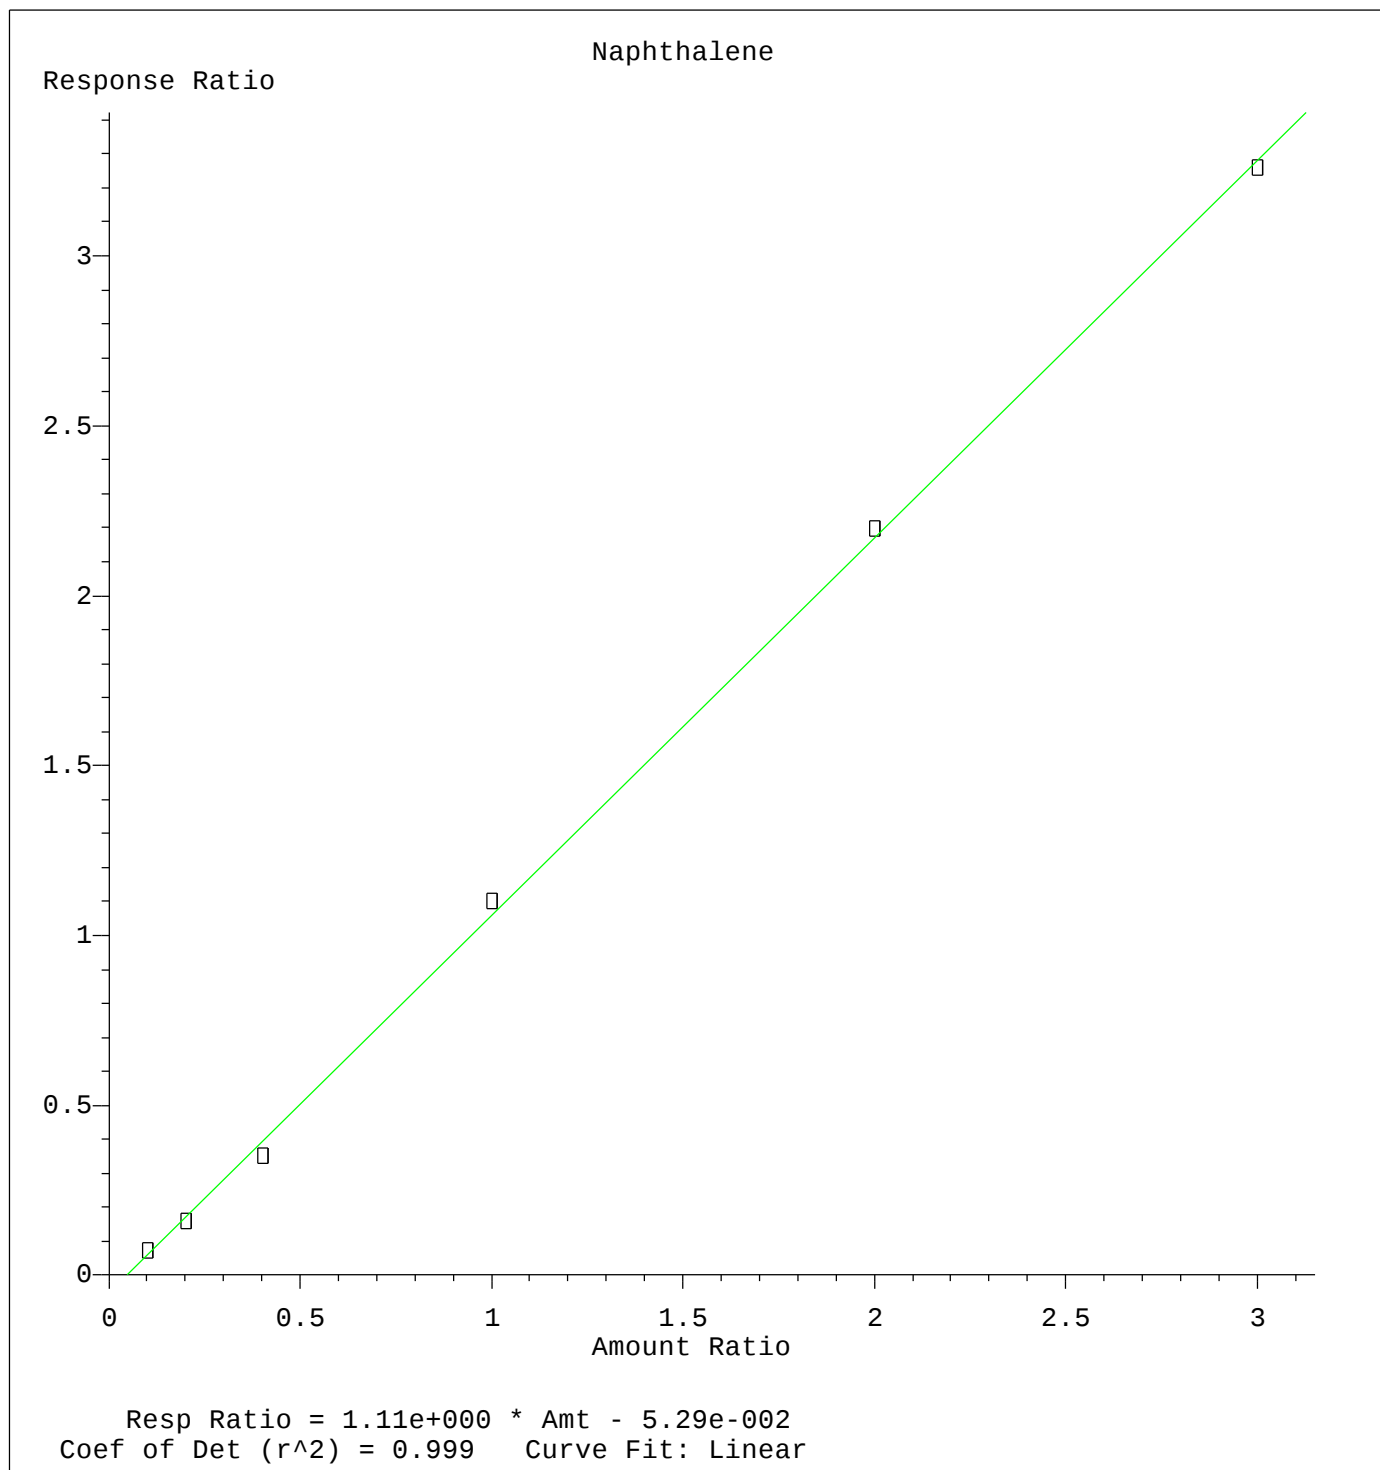

Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015

Dichlorodifluoromethane

Response Ratio

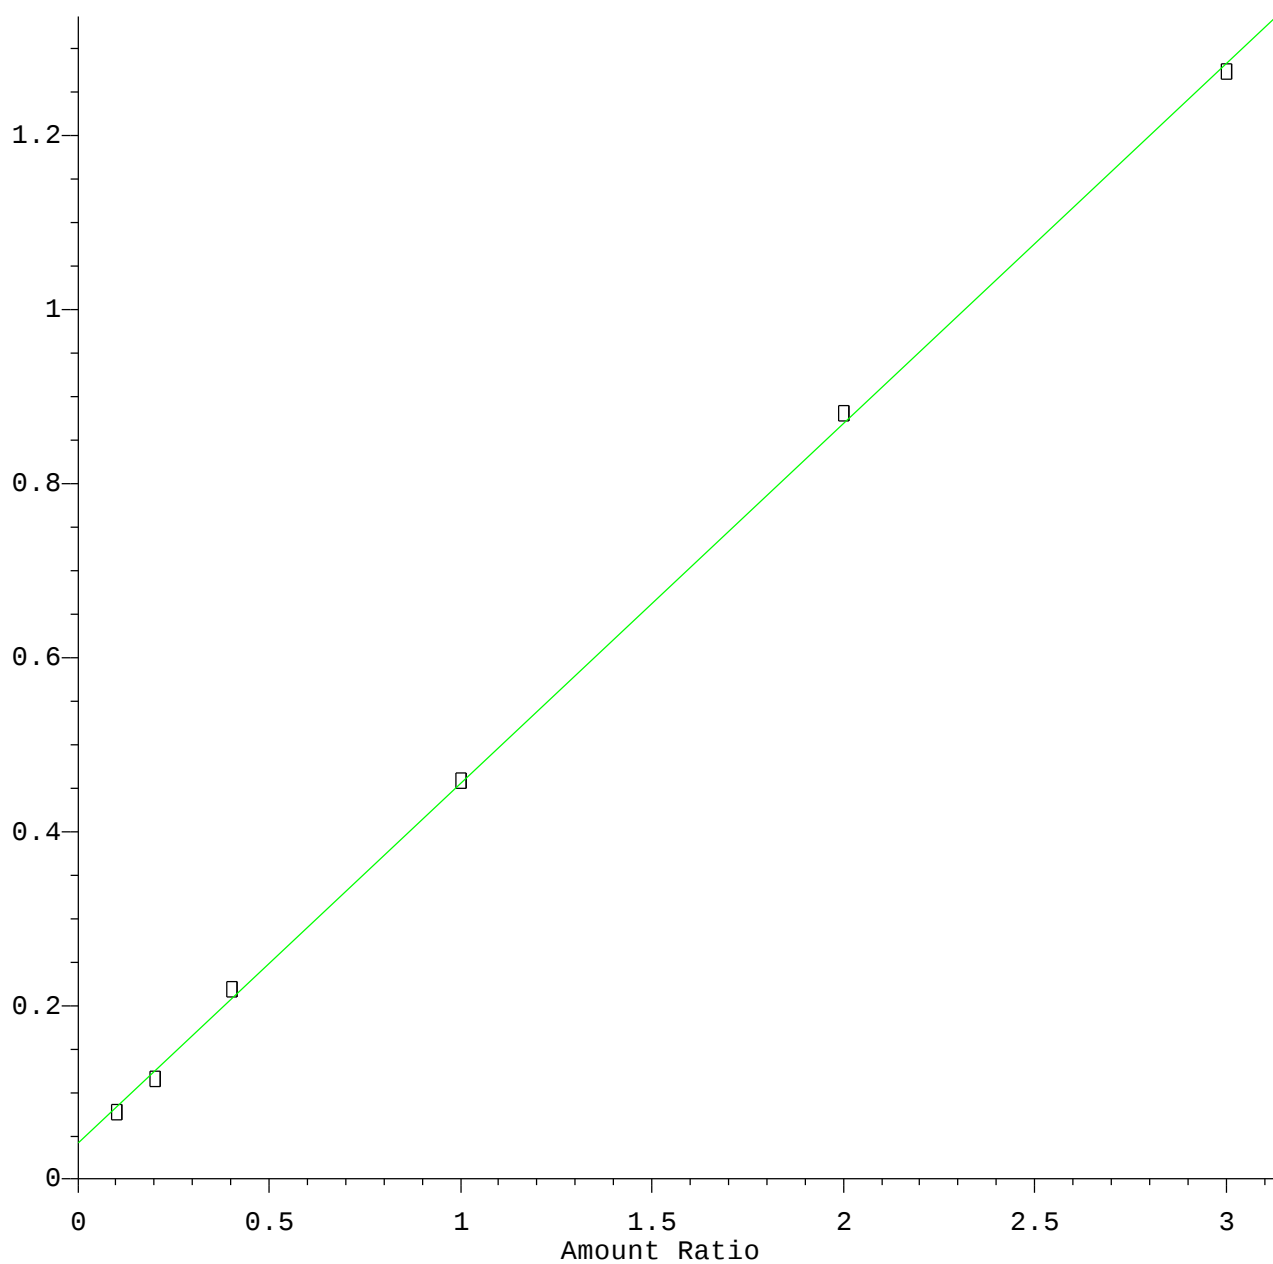

Resp Ratio = $4.14 \times 10^{-1} \times \text{Amt} + 4.12 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Calibration Table Last Updated: Fri Sep 18 15:47:18 2015