


Data Path : W:\HPCHEM1\MSVOA D\Data\VD091815\
Data File : VD046777.D
Acq On : 18 Sep 2015 10:58
Operator : FY/SY
Sample : BFB
Misc : 5.00qm/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Title : SW846 8260
Last Update : Fri Sep 18 13:41:37 2015

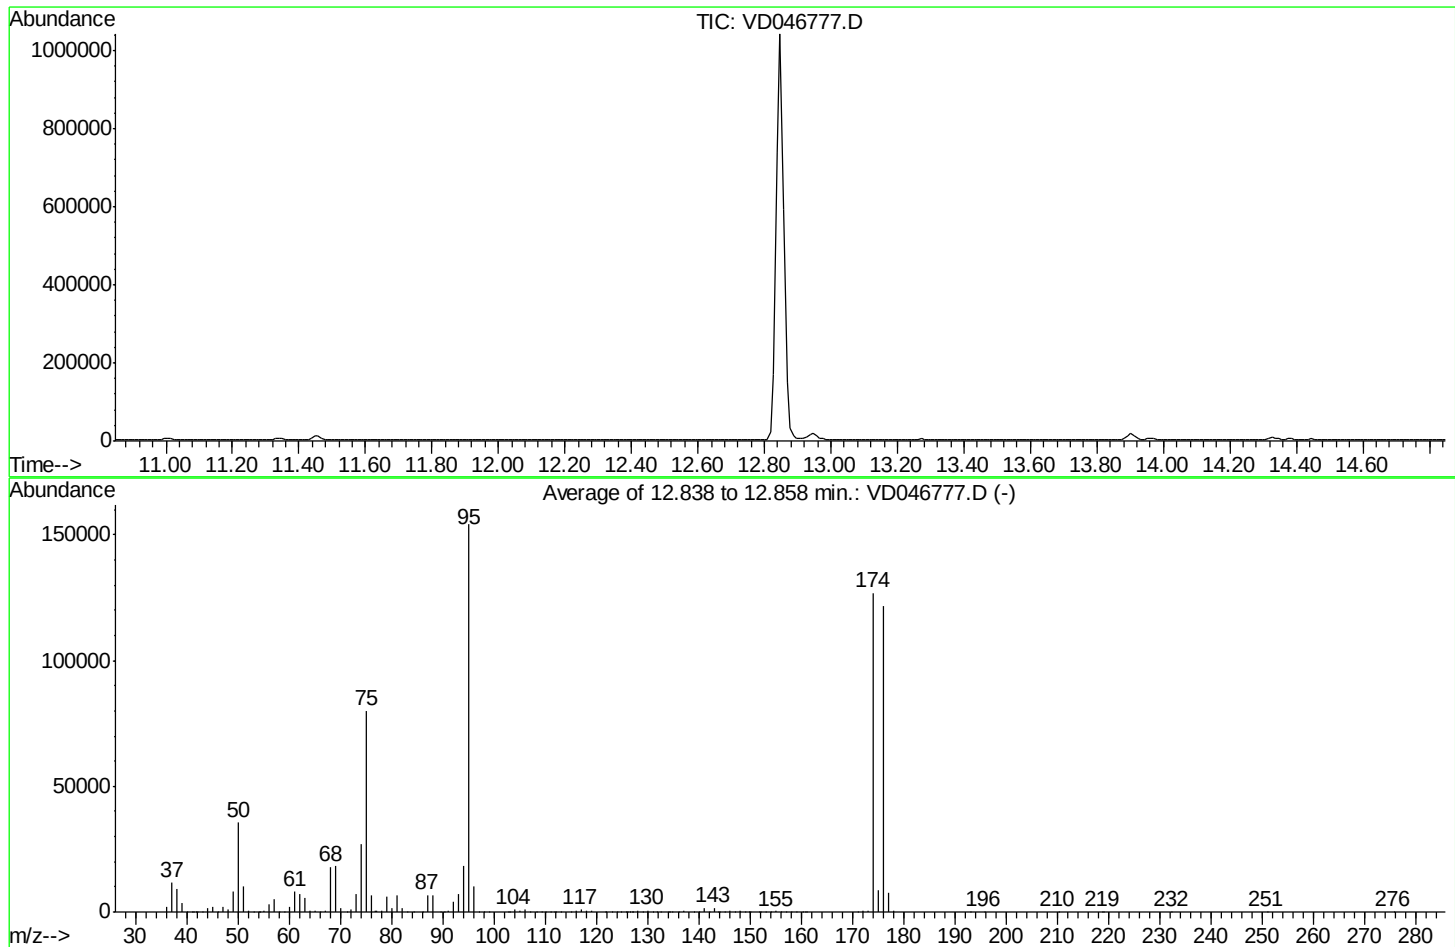

AutoFind: Scans 1249, 1250, 1251; Background Corrected with Scan 1243

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	35501	PASS
75	95	30	60	51.9	80013	PASS
95	95	100	100	100.0	154160	PASS
96	95	5	9	6.6	10140	PASS
173	174	0.00	2	0.6	721	PASS
174	95	50	100	82.2	126760	PASS
175	174	5	9	6.8	8569	PASS
176	174	95	101	95.9	121600	PASS
177	176	5	9	6.4	7812	PASS