

Data Path : W:\HPCHEM1\MSVOA D\DATA\VD092115\
 Data File : VD046799.D
 Acq On : 21 Sep 2015 11:41
 Operator : FY/SY
 Sample : VD0921SBL01
 Misc : 5.00gm/5mL/MSVOA D/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0921SBL01

Quant Time: Sep 22 01:32:05 2015
 Quant Method : W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
 Quant Title : SW846 8260
 QLast Update : Fri Sep 18 15:47:18 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	6.29	168	184801	50.00	ug/l	-0.01
34) 1,4-Difluorobenzene	7.42	114	247354	50.00	ug/l	-0.01
63) Chlorobenzene-d5	11.56	117	232908	50.00	ug/l	-0.02
72) 1,4-Dichlorobenzene-d4	13.90	152	116381	50.00	ug/l	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.70	65	108559	56.50	ug/l	-0.01
Spiked Amount				50.000		
Recovery						= 113.00%
35) Dibromofluoromethane	6.20	113	103738	53.60	ug/l	-0.02
Spiked Amount				50.000		
Recovery						= 107.20%
50) Toluene-d8	9.61	98	327772	53.69	ug/l	-0.01
Spiked Amount				50.000		
Recovery						= 107.38%
62) 4-Bromofluorobenzene	12.84	95	126454	51.44	ug/l	-0.01
Spiked Amount				50.000		
Recovery						= 102.88%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
21) Methylene Chloride	3.49	84	2839	1.61	ug/l	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA D\DATA\VD092115\
Data File : VD046799.D
Acq On : 21 Sep 2015 11:41
Operator : FY/SY
Sample : VD0921SBL01
Misc : 5.00qm/5mL/MSVOA D/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0921SBL01

Quant Time: Sep 22 01:32:05 2015
Quant Method : W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Quant Title : SW846 8260
QLast Update : Fri Sep 18 15:47:18 2015
Response via : Initial Calibration

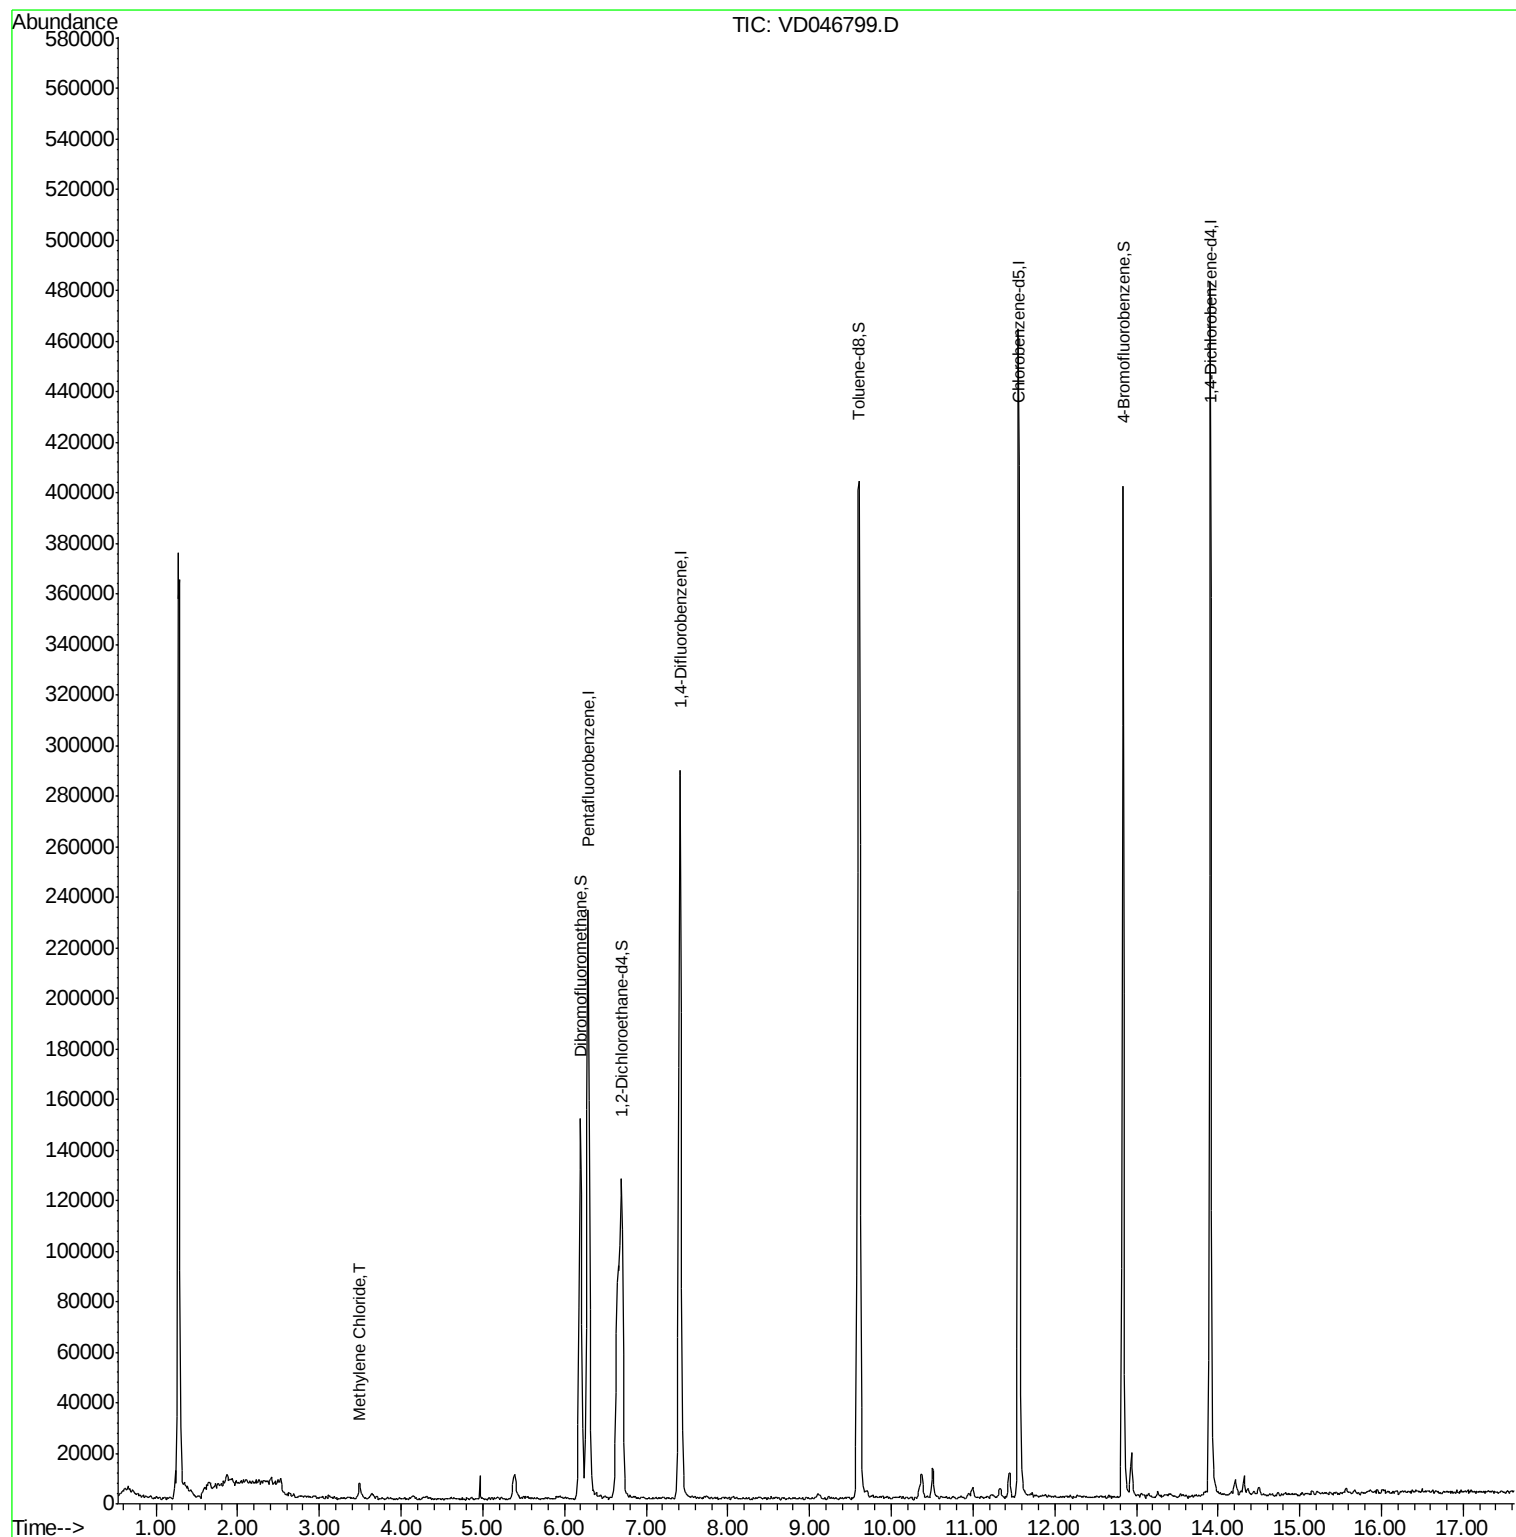

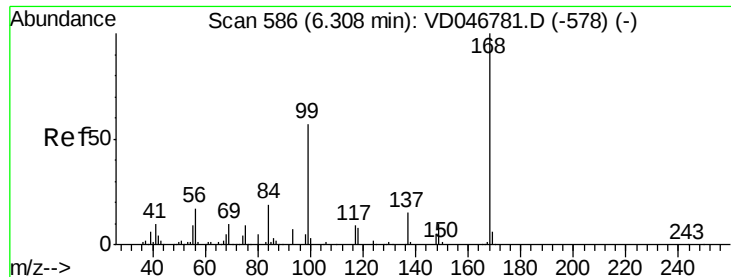

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 6.29 min Scan# 585

Delta R.T. -0.01 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41

Instrument :

MSVOA_D

ClientSampleId :


VD0921SBL01

Tot Ion:168 Resp: 184801

Ion Ratio Lower Upper




168 100

99 58.6 42.4 63.6

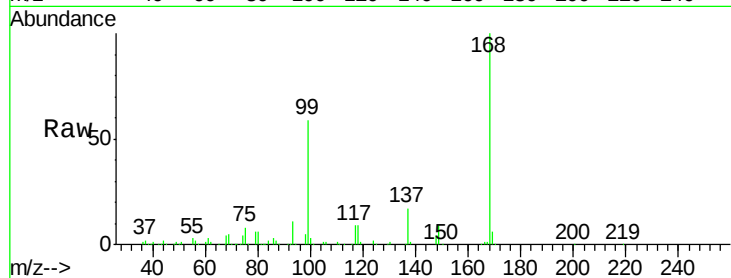

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

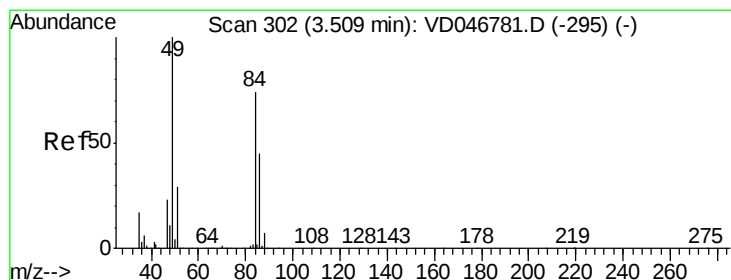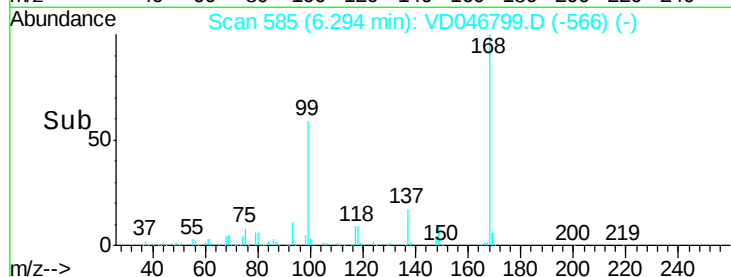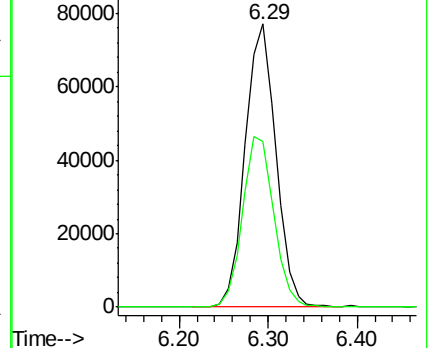

#21

Methylene Chloride

Concen: 1.61 ug/l

RT: 3.49 min Scan# 301

Delta R.T. -0.01 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41

Tgt Ion: 84 Resp: 2839


Ion Ratio Lower Upper

84 100

49 123.0 122.1 183.1

51 48.5 33.6 50.4

86 57.7 48.3 72.5


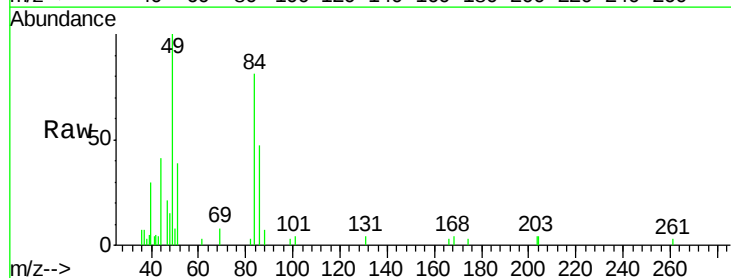



Abundance Ion 83.95 (83.65 to 84.65): VDC

Ion 48.90 (48.60 to 49.60): VDC

Ion 50.90 (50.60 to 51.60): VDC

Ion 85.90 (85.60 to 86.60): VDC



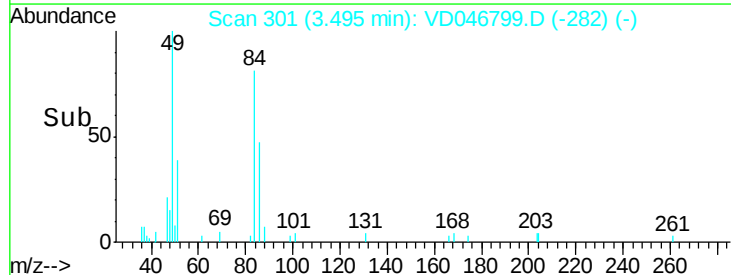
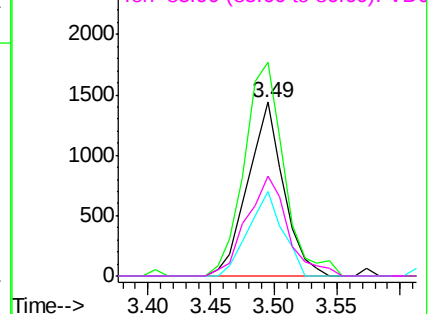


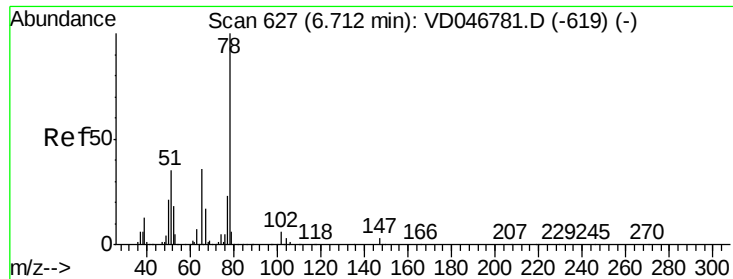

#33
 1,2-Dichloroethane-d4
 Concen: Below ug/l
 RT: 6.70 min Scan# 626
 Delta R.T. -0.01 min
 Lab File: VD046799.D
 Acq: 21 Sep 2015 11:41




Instrument :
 MSVOA_D
 ClientSampleId :
 VD0921SBL01


Tot Ion: 65 Resp: 108559
 Ion Ratio Lower Upper
 65 100
 67 46.3 0.0 105.4

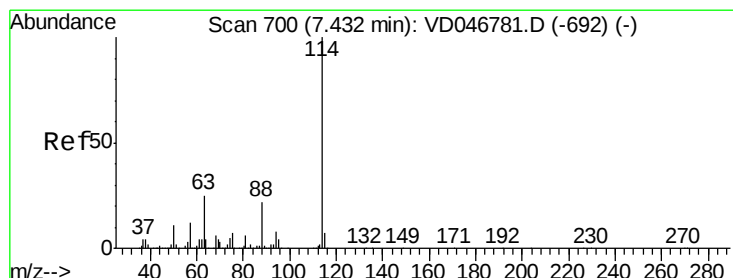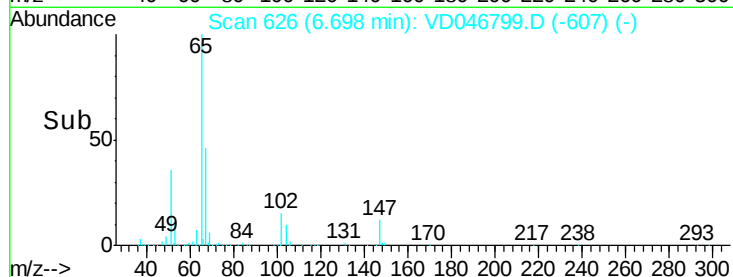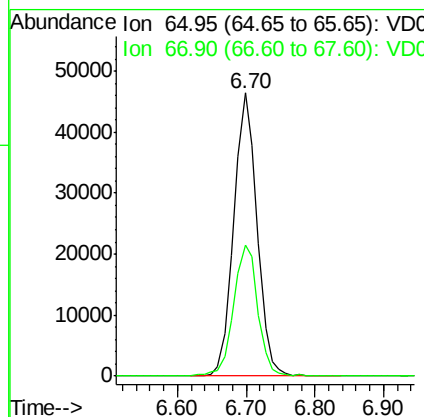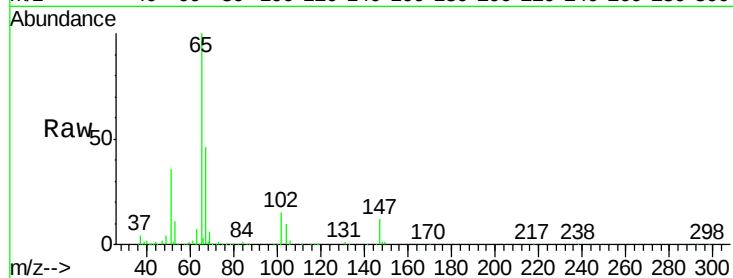

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 7.42 min Scan# 699
 Delta R.T. -0.01 min
 Lab File: VD046799.D
 Acq: 21 Sep 2015 11:41

Tgt Ion: 114 Resp: 247354
 Ion Ratio Lower Upper
 114 100
 63 23.5 0.0 49.8
 88 21.8 0.0 43.6

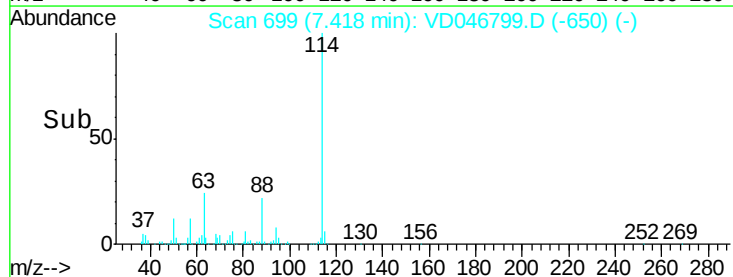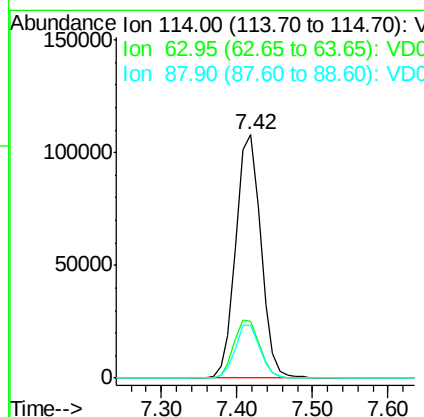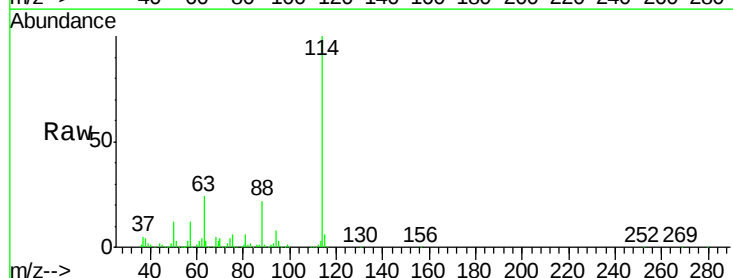

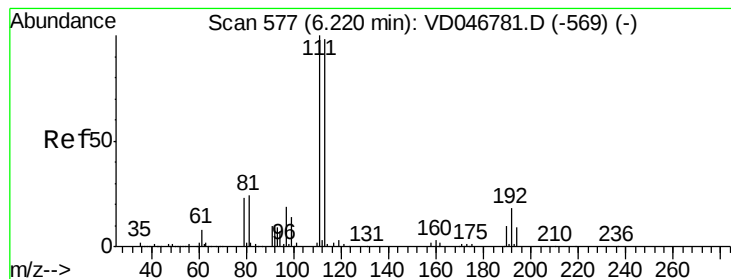

#35

Dibromofluoromethane

Concen: 50.00 ug/l

RT: 6.20 min Scan# 575

Delta R.T. -0.02 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41

Instrument :

MSVOA_D

ClientSampleId :

VD0921SBL01


Tot Ion:113 Resp: 103738

Ion Ratio Lower Upper

113 100

111 98.5 79.4 119.0




192 19.8 14.6 22.0

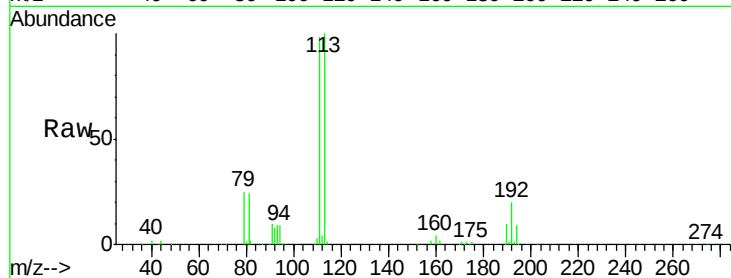

Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

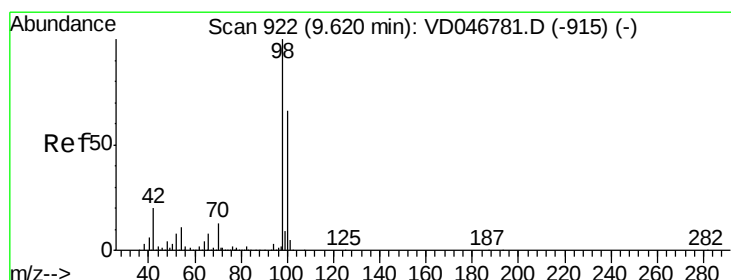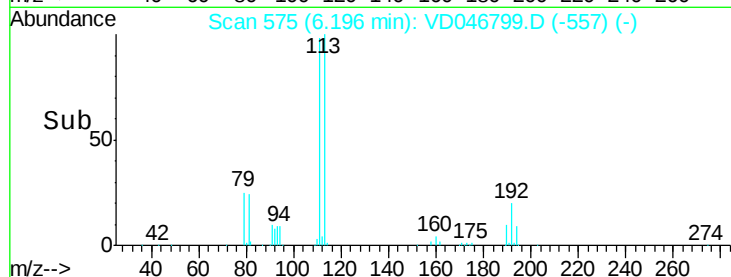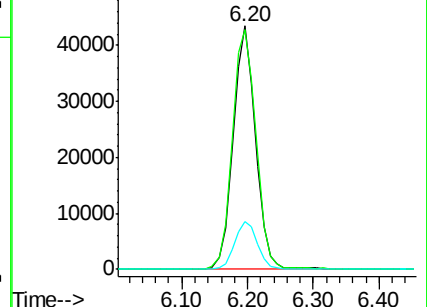

#50

Toluene-d8

Concen: N.D. ug/l

RT: 9.61 min Scan# 921

Delta R.T. -0.01 min

Lab File: VD046799.D


Acq: 21 Sep 2015 11:41

Tgt Ion: 98 Resp: 327772

Ion Ratio Lower Upper



98 100


100 66.5 49.9 74.9

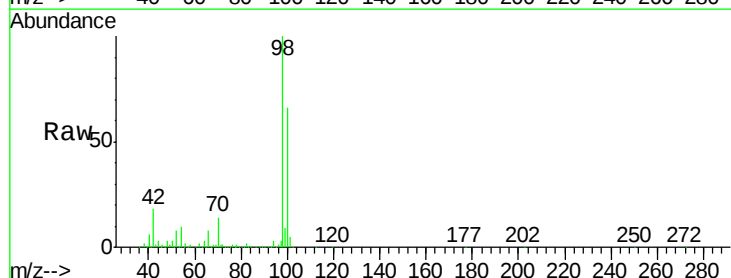

Abundance Ion 98.05 (97.75 to 98.75): V

Ion 100.05 (99.75 to 100.75): V

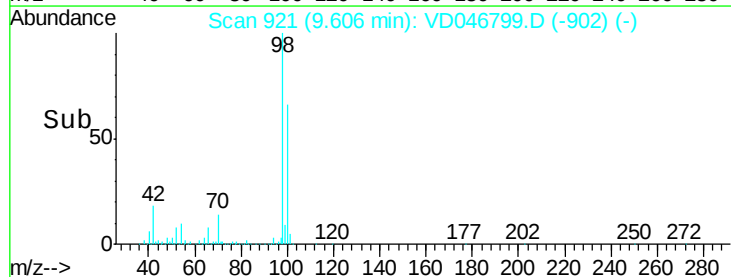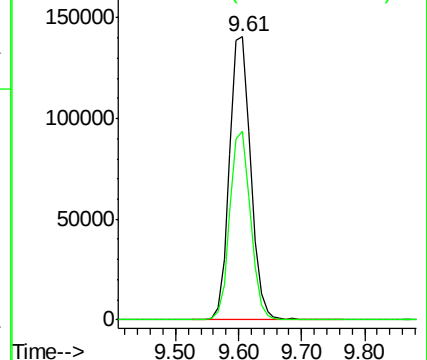

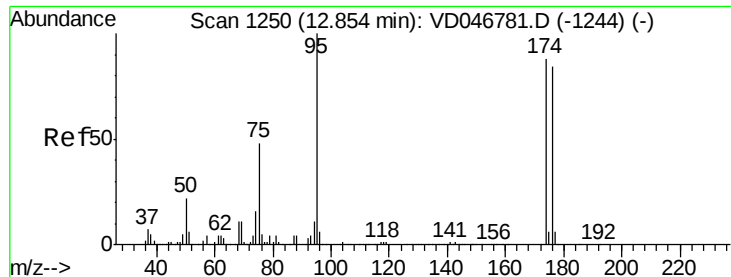

#62

4-Bromofluorobenzene

Concen: Below ug/l

RT: 12.84 min Scan# 1249

Delta R.T. -0.01 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41

Instrument :

MSVOA_D

ClientSampleId :

VD0921SBL01


Tot Ion: 95 Resp: 126454

Ion Ratio Lower Upper

95 100

174 84.4 0.0 149.8

176 80.5 0.0 143.4

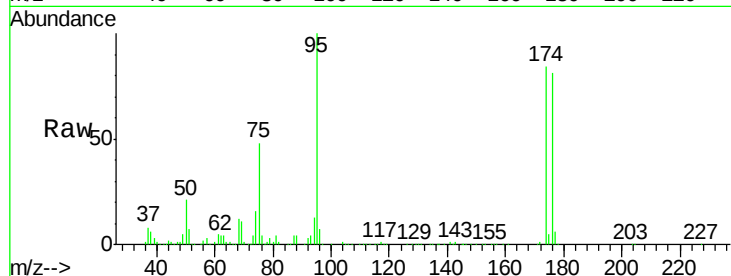


Abundance Ion 95.00 (94.70 to 95.70): VD046781.D (-1244) (-)

Ion 173.90 (173.60 to 174.60): VD046781.D (-1244) (-)


Ion 175.90 (175.60 to 176.60): VD046781.D (-1244) (-)

12.84

Time-->

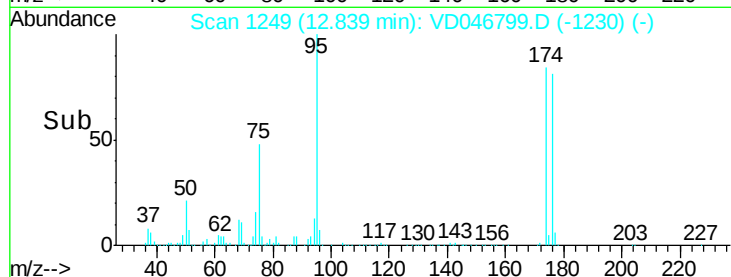

Time-->

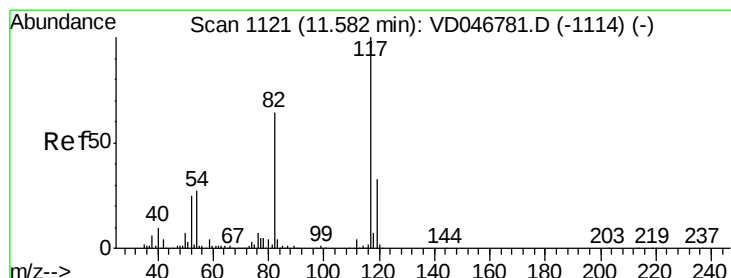

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.56 min Scan# 1119

Delta R.T. -0.02 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41


Tgt Ion: 117 Resp: 232908

Ion Ratio Lower Upper

117 100

82 71.4 50.6 75.8

119 31.9 25.8 38.8

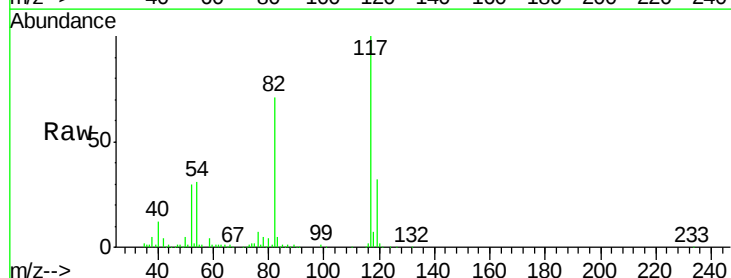


Abundance Ion 116.95 (116.65 to 117.65): VD046781.D (-1114) (-)

Ion 82.05 (81.75 to 82.75): VD046781.D (-1114) (-)


Ion 118.95 (118.65 to 119.65): VD046781.D (-1114) (-)

11.56

Time-->

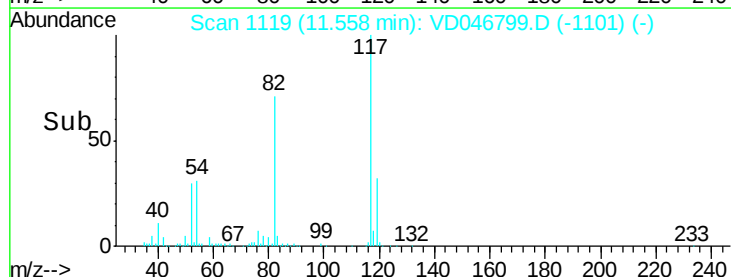

Time-->

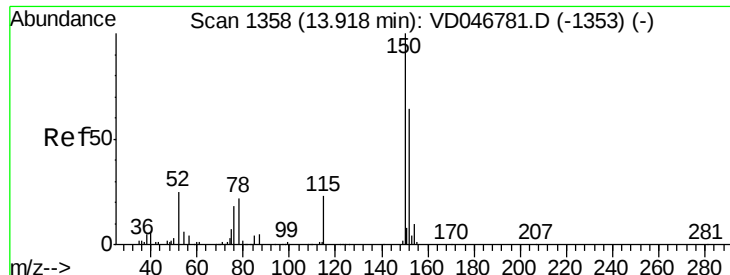

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.90 min Scan# 1357

Delta R.T. -0.01 min

Lab File: VD046799.D

Acq: 21 Sep 2015 11:41

Instrument :

MSVOA_D

ClientSampleId :

VD0921SBL01


Tot Ion:152 Resp: 116381

Ion Ratio Lower Upper

152 100

115 56.0 26.2 78.6

150 158.2 0.0 311.8

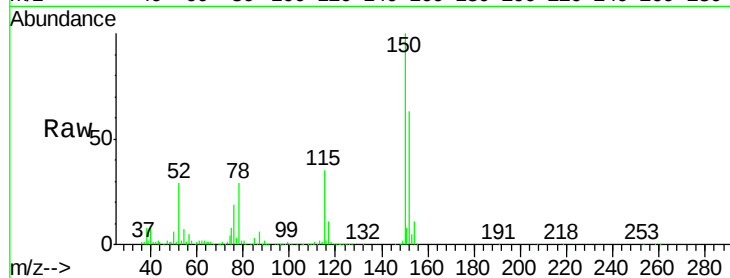

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 115.00 (114.70 to 115.70): V

Ion 149.90 (149.60 to 150.60): V

