


Data Path : W:\HPCHEM1\MSVOA D\DATA\VD092115\
Data File : VD046797.D
Acq On : 21 Sep 2015 9:56
Operator : FY/SY
Sample : BFB
Misc : 5.00qm/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Title : SW846 8260
Last Update : Fri Sep 18 15:47:18 2015

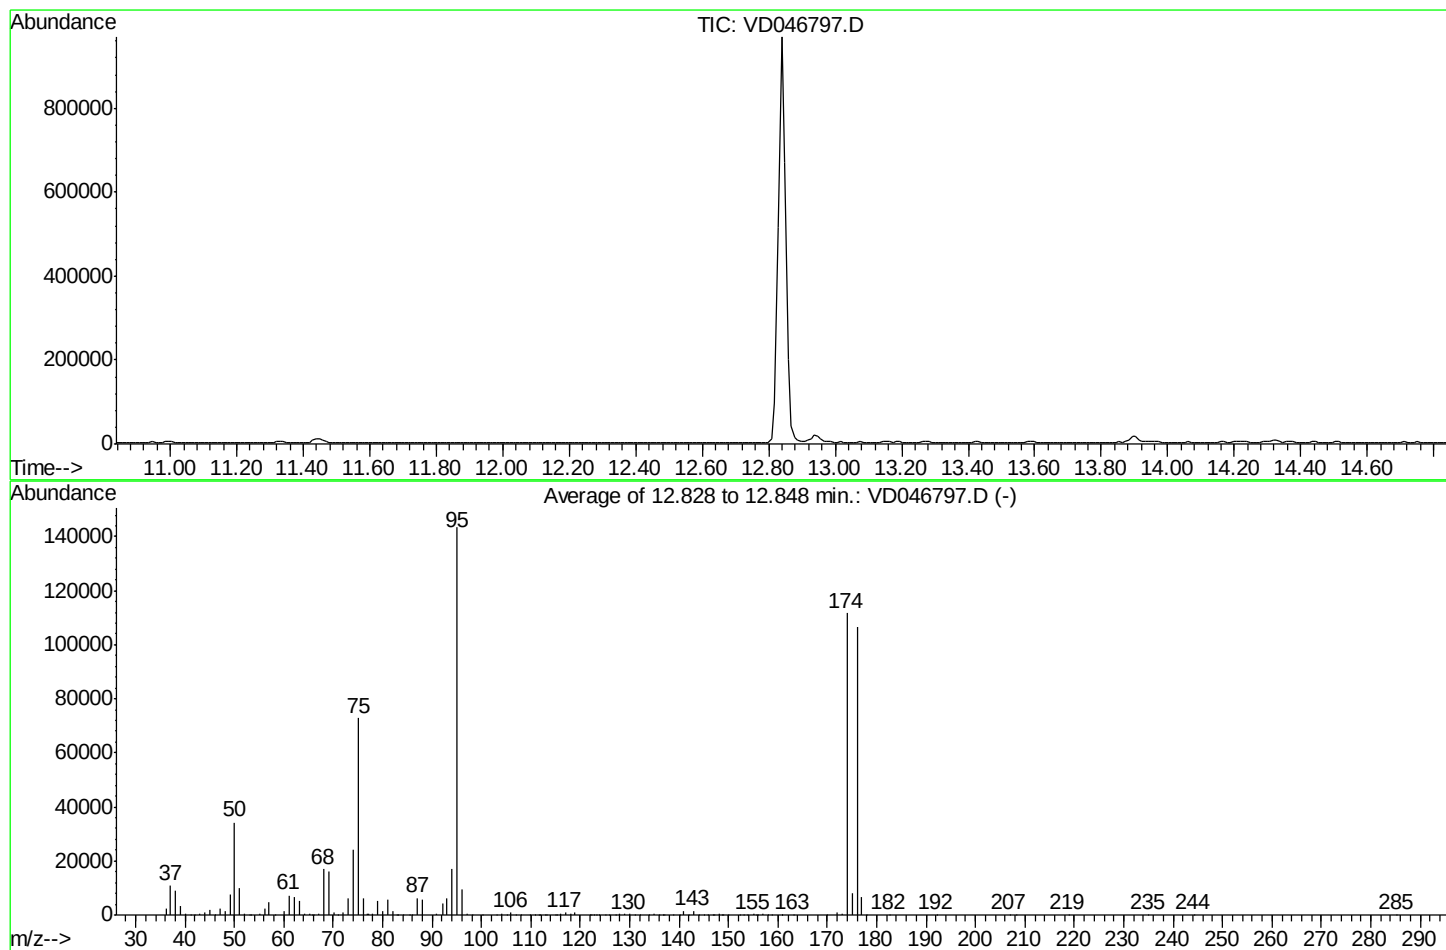

AutoFind: Scans 1248, 1249, 1250; Background Corrected with Scan 1242

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	34104	PASS
75	95	30	60	50.8	72840	PASS
95	95	100	100	100.0	143442	PASS
96	95	5	9	6.5	9265	PASS
173	174	0.00	2	0.4	401	PASS
174	95	50	100	77.8	111626	PASS
175	174	5	9	7.2	8037	PASS
176	174	95	101	95.4	106456	PASS
177	176	5	9	6.3	6750	PASS