
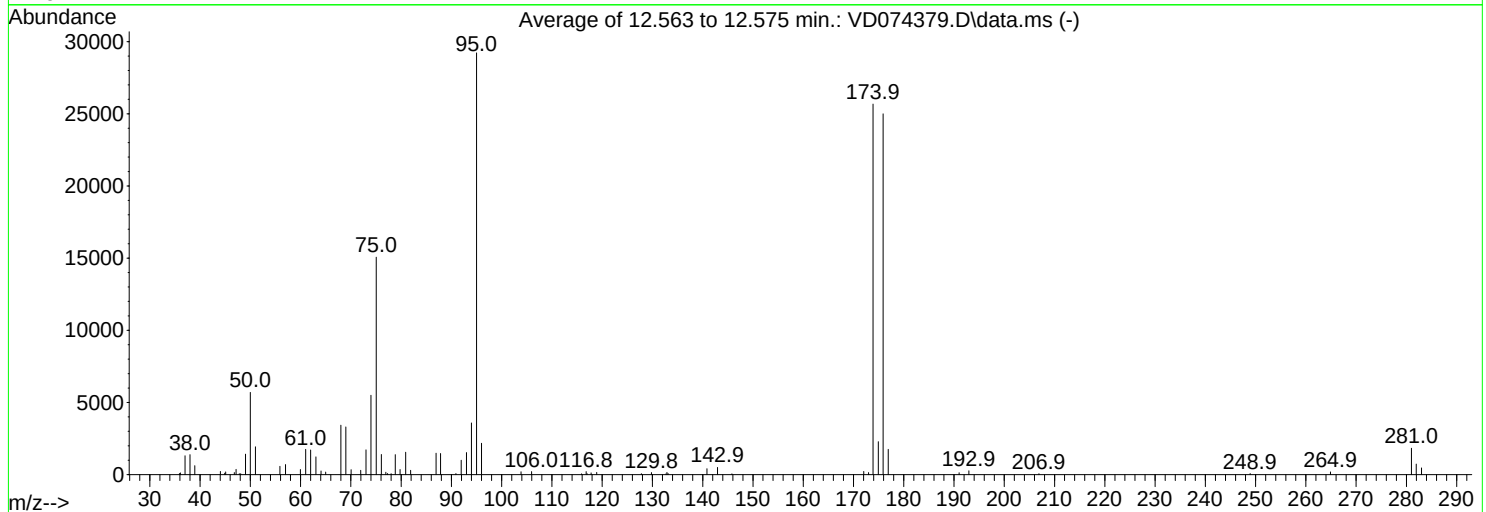


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092122\
Data File : VD074379.D
Acq On : 21 Sep 2022 09:06
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D091622S.M
Title : SW846 8260
Last Update : Sat Sep 17 04:16:54 2022

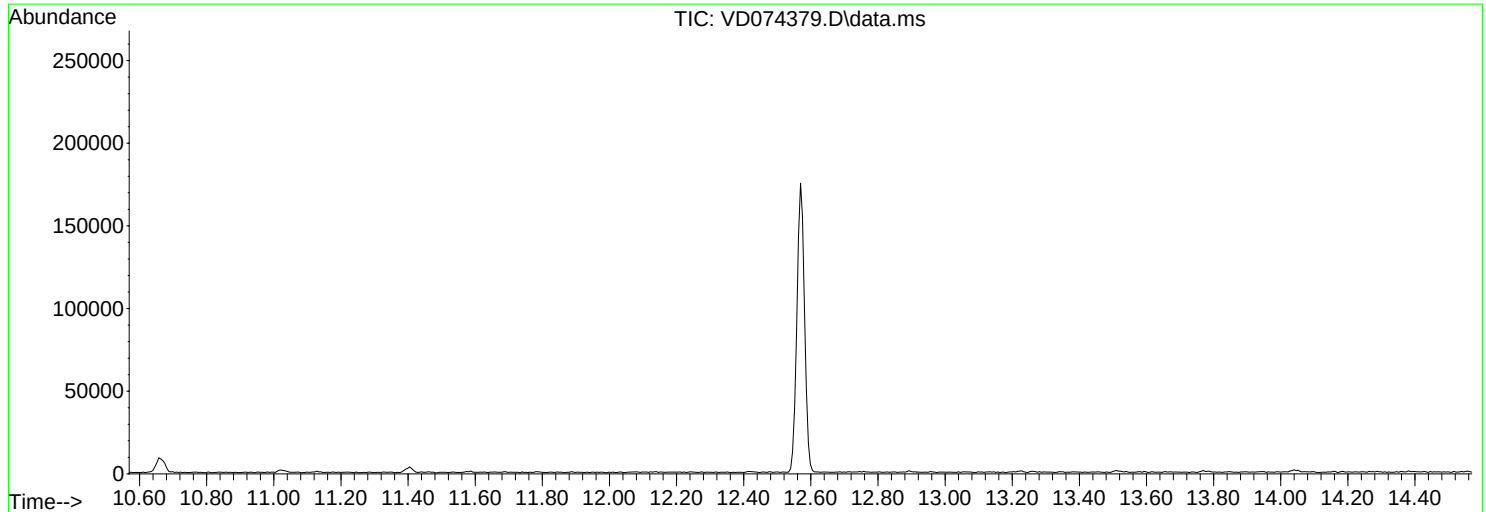

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	5703	PASS
75	95	30	60	51.5	15062	PASS
95	95	100	100	100.0	29221	PASS
96	95	5	9	7.4	2175	PASS
173	174	0.00	2	0.5	139	PASS
174	95	50	100	87.8	25667	PASS
175	174	5	9	8.9	2281	PASS
176	174	95	101	97.4	24992	PASS
177	176	5	9	7.0	1755	PASS