
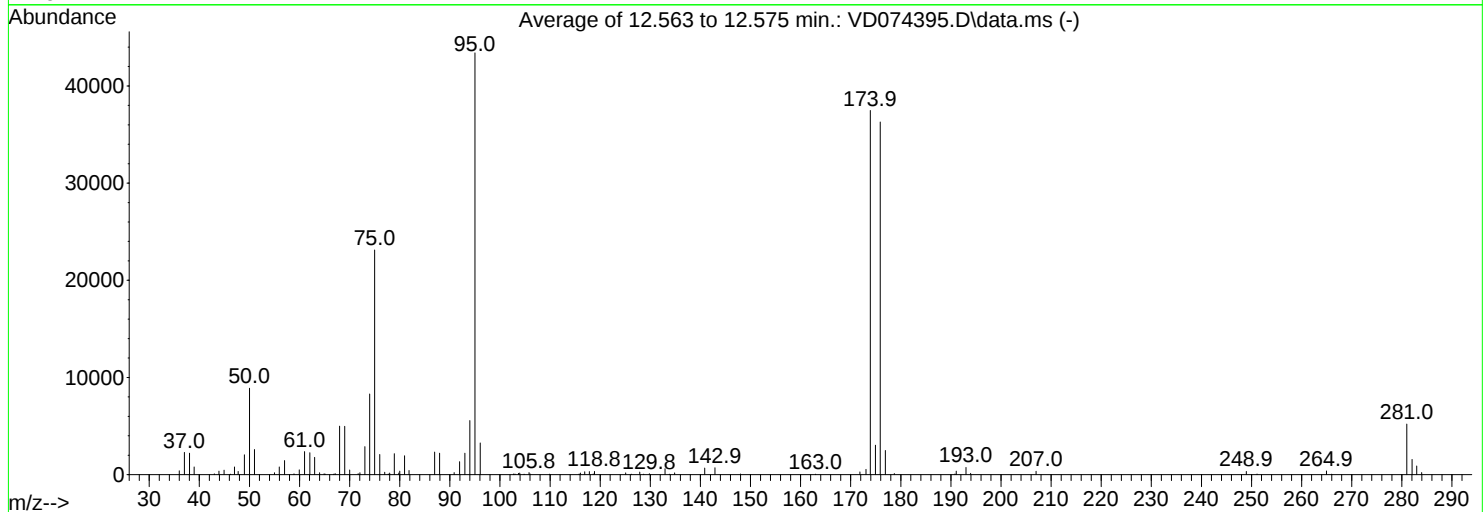


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092222\
 Data File : VD074395.D
 Acq On : 22 Sep 2022 09:16
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D092222S.M
 Title : SW846 8260
 Last Update : Fri Sep 23 08:08:51 2022

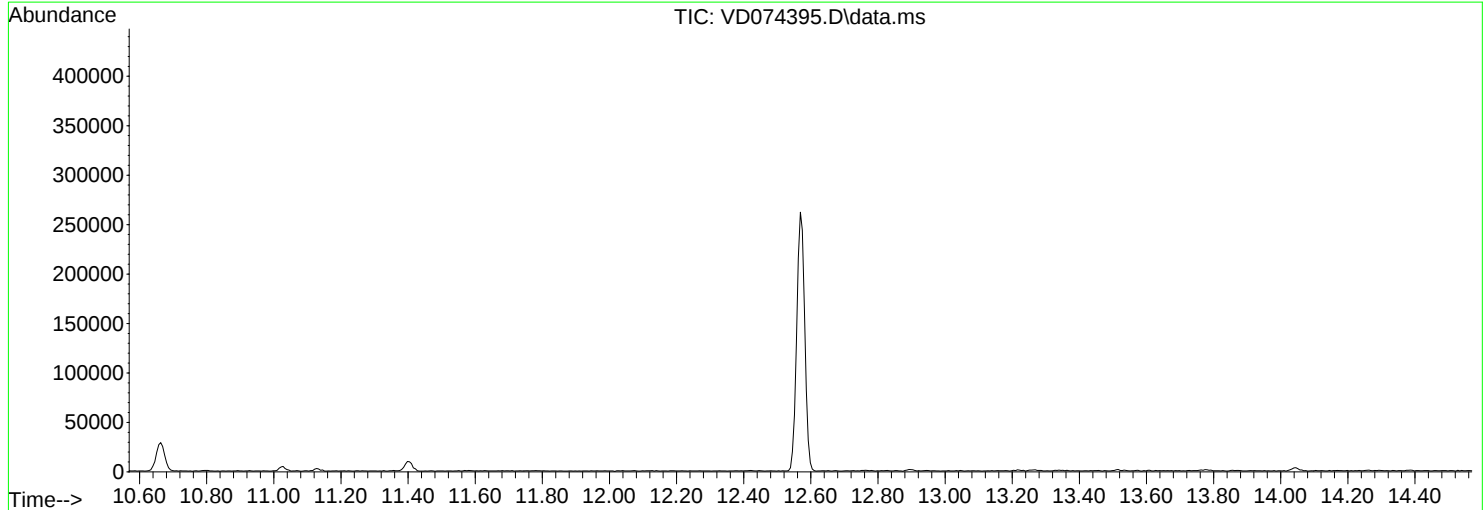

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	8890	PASS
75	95	30	60	53.3	23120	PASS
95	95	100	100	100.0	43408	PASS
96	95	5	9	7.5	3265	PASS
173	174	0.00	2	1.5	547	PASS
174	95	50	100	86.3	37475	PASS
175	174	5	9	8.1	3035	PASS
176	174	95	101	96.8	36291	PASS
177	176	5	9	6.9	2487	PASS