


Data Path : W:\HPCHEM1\MSVOA D\DATA\VD092315\
Data File : VD046847.D
Acq On : 23 Sep 2015 10:06
Operator : FY/SY
Sample : BFB
Misc : 5.00qm/5mL/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_D\METHOD\82D091815S.M
Title : SW846 8260
Last Update : Fri Sep 18 15:47:18 2015

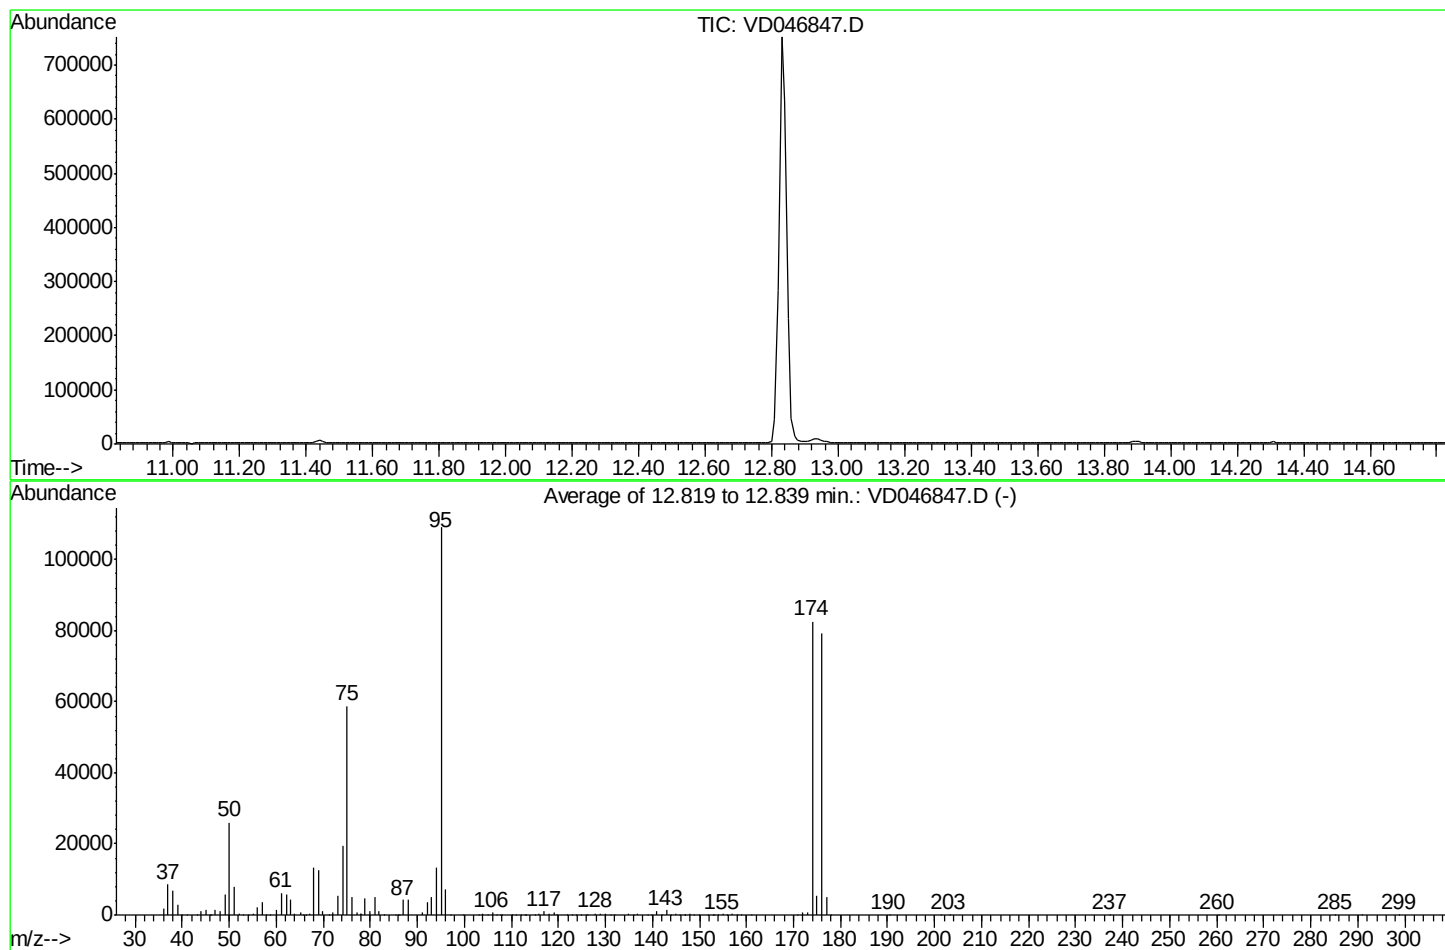

AutoFind: Scans 1247, 1248, 1249; Background Corrected with Scan 1242

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	26002	PASS
75	95	30	60	53.9	58770	PASS
95	95	100	100	100.0	109050	PASS
96	95	5	9	6.5	7045	PASS
173	174	0.00	2	0.7	593	PASS
174	95	50	100	75.7	82602	PASS
175	174	5	9	6.7	5537	PASS
176	174	95	101	95.9	79256	PASS
177	176	5	9	6.6	5224	PASS