

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092424\
 Data File : VD079878.D
 Acq On : 24 Sep 2024 15:50
 Operator : RP/MD
 Sample : P4162-08
 Misc : 4.82G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4ES7

Quant Time: Sep 25 01:23:55 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Sep 25 01:21:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	217272	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	141429	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	26617	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	163743	17.331	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.320%
7) Chloroethane-d5	2.799	69	157075	20.999	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.000%
11) 1,1-Dichloroethene-d2	3.917	65	28096	16.379	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.520%
21) 2-Butanone-d5	6.987	46	16160	18.410	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	36.820%
24) Chloroform-d	7.563	84	129279	18.101	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.400%
26) 1,2-Dichloroethane-d4	8.228	65	68075	18.228	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.920%
32) Benzene-d6	8.205	84	256413	25.680	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	102.720%
36) 1,2-Dichloropropane-d6	9.210	67	84361	27.587	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.360%
41) Toluene-d8	10.269	98	180903	20.589	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.360%
43) trans-1,3-Dichloroprop...	10.522	79	23170	17.623	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.480%
47) 2-Hexanone-d5	10.875	63	13471	27.023	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	54.040%
56) 1,1,2,2-Tetrachloroeth...	12.645	84	34387	15.302	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	61.200%
66) 1,2-Dichlorobenzene-d4	13.810	152	18467	18.397	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	73.600%#
Target Compounds						Qvalue
16) Methylene chloride	4.805	84	22649	5.276	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092424\
Data File : VD079878.D
Acq On : 24 Sep 2024 15:50
Operator : RP/MD
Sample : P4162-08
Misc : 4.82G/10ml/MSVOA_D/SOIL/A
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4ES7


Quant Time: Sep 25 01:23:55 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Sep 25 01:21:43 2024
Response via : Initial Calibration

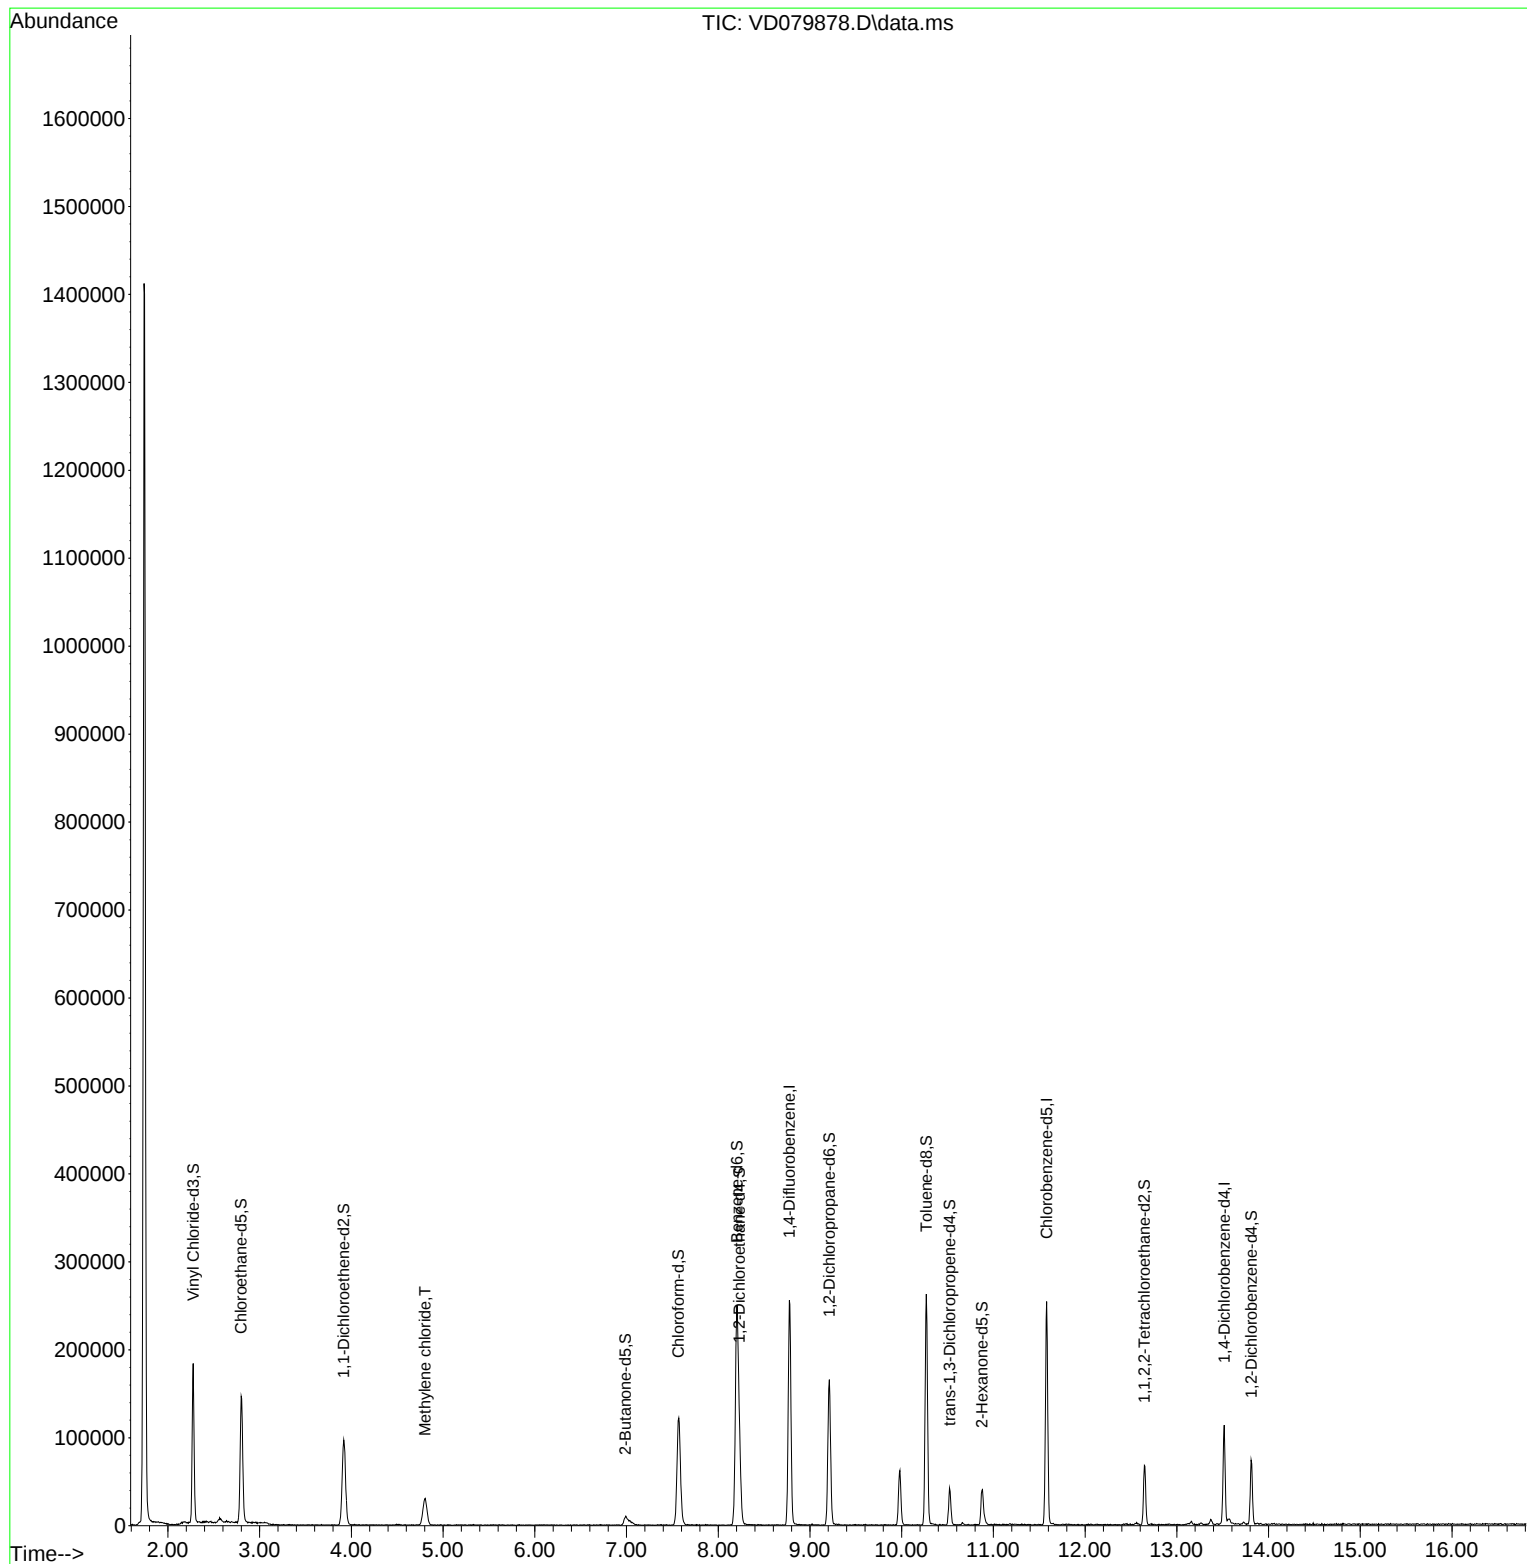

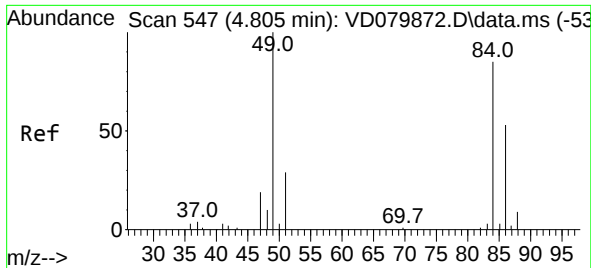

#16
Methylene chloride
Concen: 5.276 ug/L
RT: 4.805 min Scan# 54
Delta R.T. -0.000 min
Lab File: VD079878.D
Acq: 24 Sep 2024 15:50

Instrument :
MSVOA_D
ClientSampleId :
A4ES7

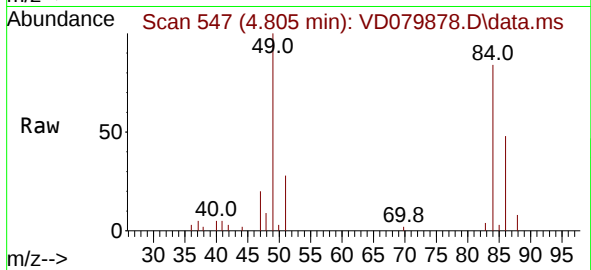

Tgt Ion: 84 Resp: 22649
Ion Ratio Lower Upper
84 100
86 57.1 41.0 76.2
49 119.7 90.0 167.2

