
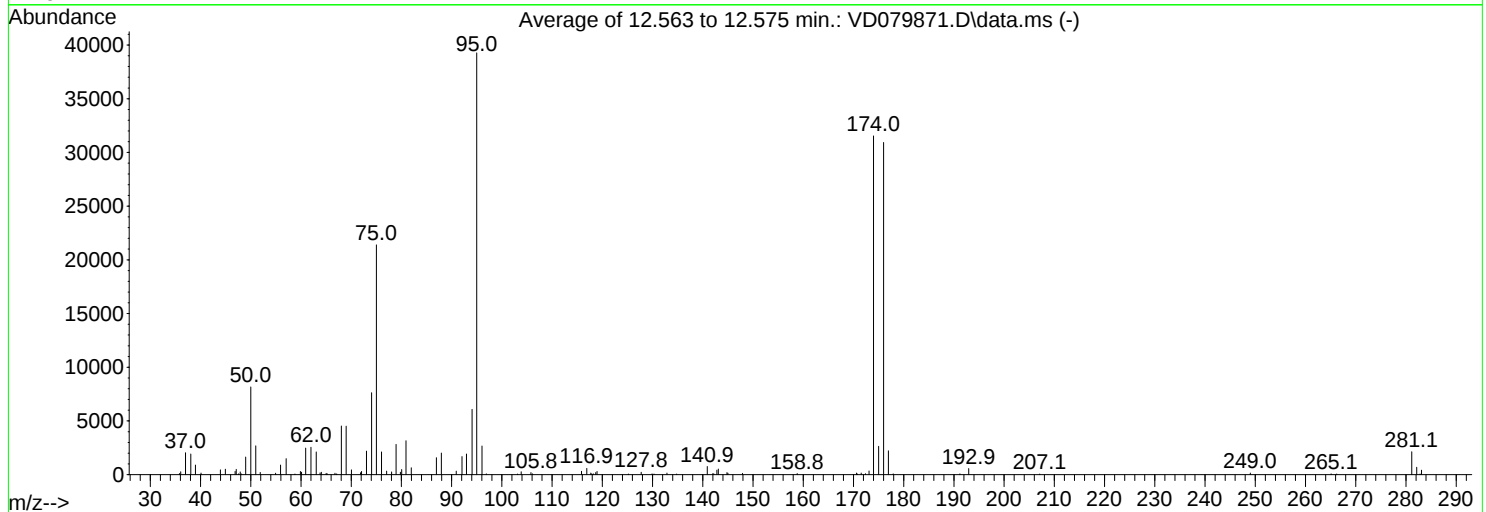


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092424\
Data File : VD079871.D
Acq On : 24 Sep 2024 09:20
Operator : RP/MD
Sample : BFB832
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB832

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Wed Sep 25 01:21:43 2024

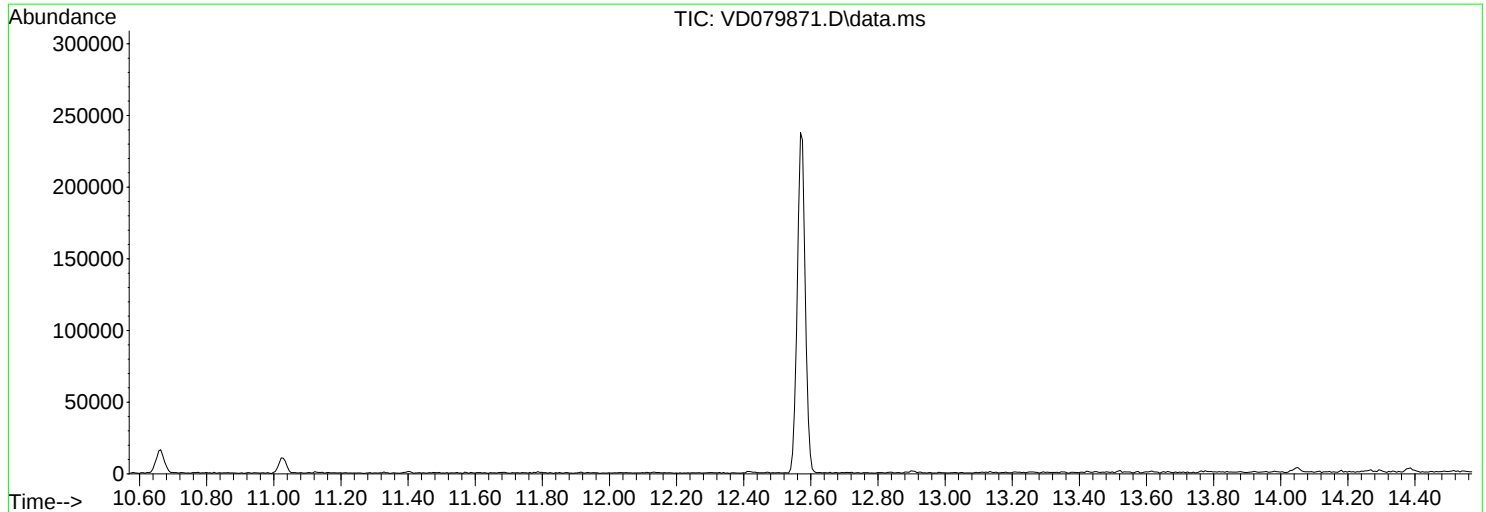

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	8167	PASS
75	95	30	80	54.5	21389	PASS
95	95	100	100	100.0	39272	PASS
96	95	5	9	6.8	2660	PASS
173	174	0.00	2	1.1	338	PASS
174	95	50	120	80.3	31541	PASS
175	174	5	9	8.3	2633	PASS
176	174	95	105	98.1	30933	PASS
177	176	5	10	7.2	2223	PASS

m/z	Abundance
36.40	160.0
39.90	623.0

Instrument :
MSVOA_D
ClientSampleId :
BFB832

m/z	Abundance
35.80	339.0
37.00	1758.0
38.00	1578.0
39.10	622.0
39.90	422.0
43.90	409.0
45.10	510.0
46.90	899.0
48.00	383.0
49.00	1159.0
50.00	6919.0
51.00	2212.0
51.90	240.0
55.00	224.0
55.90	872.0
57.10	1016.0
59.90	387.0
60.90	1939.0
62.00	2402.0
63.10	2238.0
64.00	277.0
65.00	192.0
67.10	221.0
68.00	4394.0
69.00	3730.0
70.00	458.0
71.90	158.0
73.10	2042.0
74.10	5810.0
75.00	18272.0
76.00	1696.0
77.10	323.0
78.00	171.0
79.00	2276.0
79.80	687.0
80.90	2589.0
81.90	413.0
86.90	1195.0
87.90	1611.0
90.90	268.0
92.00	1809.0
92.90	1636.0
94.10	4745.0
95.00	33960.0
96.10	2439.0
96.90	223.0
103.10	195.0
104.00	189.0
106.10	234.0
115.90	277.0
116.80	341.0
117.70	190.0
119.00	528.0
125.20	191.0
127.70	207.0
134.80	171.0
140.90	750.0
143.10	687.0
144.80	336.0
147.90	176.0
170.60	303.0
172.40	279.0
174.00	24680.0
175.00	1942.0
176.00	23584.0
176.90	2148.0
193.00	516.0
281.20	1599.0
282.10	393.0
282.80	188.0
283.20	211.0

Instrument :
MSVOA_D
ClientSampleId :
BFB832

m/z	Abundance
36.10	406.0
37.00	2383.0
38.10	1744.0
39.00	1074.0
39.80	914.0
43.90	520.0
44.90	478.0
47.10	723.0
47.80	378.0
49.00	1562.0
50.00	8514.0
51.00	2839.0
51.90	193.0
54.90	200.0
56.00	1004.0
57.00	1627.0
58.80	179.0
59.90	505.0
61.00	2975.0
62.00	2631.0
63.00	2342.0
64.10	394.0
65.00	160.0
66.80	158.0
68.10	4733.0
69.00	5229.0
70.00	555.0
71.80	380.0
72.10	427.0
73.00	2384.0
74.10	8722.0
75.00	23504.0
76.00	2068.0
77.10	498.0
78.10	365.0
78.90	3090.0
80.10	847.0
80.90	3572.0
82.00	631.0
86.90	1603.0
88.00	2512.0
90.80	225.0
91.00	225.0
92.00	1807.0
93.00	2368.0
94.00	6382.0
95.00	42320.0
96.10	3214.0
103.80	327.0
105.80	337.0
115.80	336.0
116.90	691.0
117.70	259.0
118.20	247.0
118.70	596.0
127.80	280.0
130.30	165.0
132.80	161.0
140.90	763.0
142.00	337.0
142.80	1235.0
144.80	234.0
158.80	302.0
170.60	151.0
171.60	293.0
174.00	35064.0
175.00	3032.0
176.00	35344.0
177.00	2446.0
192.90	533.0
249.10	277.0
281.10	2106.0
282.10	508.0
283.00	423.0

Instrument :
MSVOA_D
ClientSampleId :
BFB832

m/z	Abundance
36.00	404.0
37.00	1992.0
38.00	2425.0
38.90	999.0
40.10	453.0
44.00	433.0
44.90	532.0
47.10	757.0
47.60	210.0
48.10	243.0
49.00	2208.0
50.00	9069.0
51.00	2996.0
51.90	200.0
55.90	828.0
57.00	1829.0
60.10	666.0
61.00	2528.0
62.00	2595.0
63.00	1783.0
63.80	499.0
65.20	292.0
66.70	225.0
68.00	4438.0
69.00	4565.0
70.10	342.0
72.00	455.0
73.10	2127.0
74.00	8346.0
75.00	22392.0
76.10	2576.0
76.90	151.0
78.10	214.0
78.90	3098.0
80.00	569.0
80.90	3327.0
82.00	858.0
87.00	1923.0
88.00	1924.0
90.90	275.0
92.10	1445.0
93.00	1747.0
94.00	7110.0
95.00	41536.0
96.00	2326.0
103.80	271.0
105.80	249.0
115.90	339.0
117.00	721.0
117.90	246.0
118.90	357.0
127.70	177.0
129.90	211.0
132.90	277.0
140.90	776.0
142.20	204.0
143.10	884.0
145.00	389.0
147.90	204.0
170.80	196.0
171.40	167.0
173.10	1013.0
174.00	34880.0
175.00	2925.0
176.00	33872.0
177.00	2075.0
177.90	221.0
191.20	248.0
193.00	651.0
207.10	177.0
248.90	188.0
265.10	215.0
266.20	168.0
281.20	2712.0
282.20	1152.0
283.20	605.0

Instrument :
MSVOA_D
ClientSampleId :
BFB832