
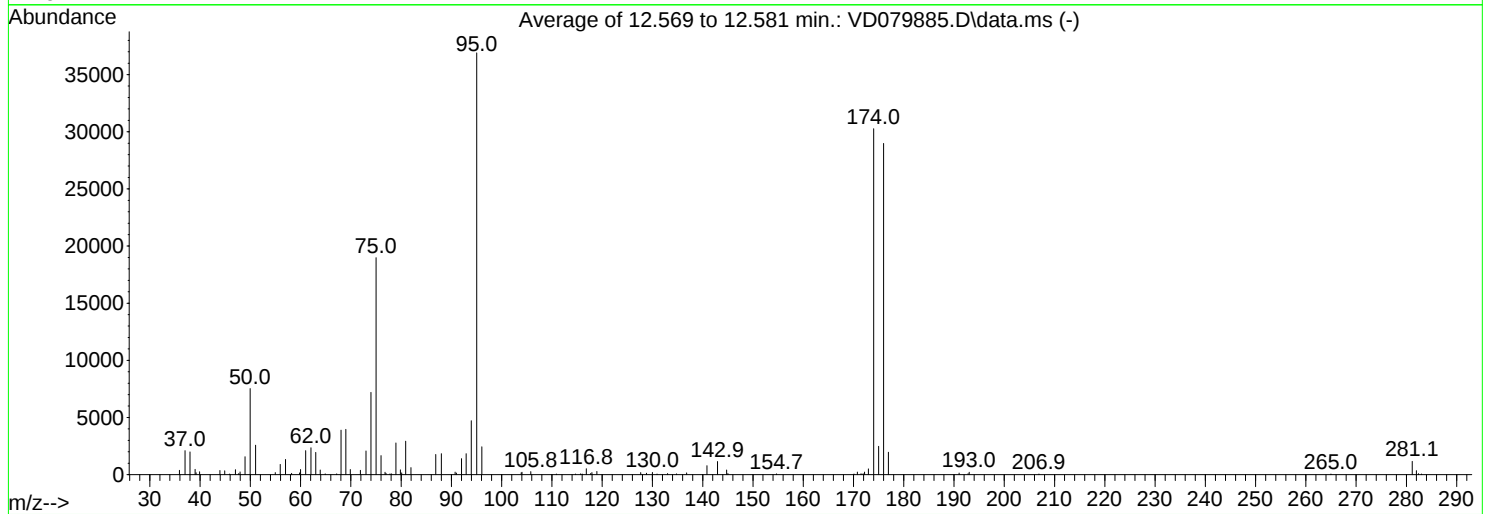


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092524\
Data File : VD079885.D
Acq On : 25 Sep 2024 09:16
Operator : RP/MD
Sample : BFB833
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB833

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Thu Sep 26 01:54:46 2024

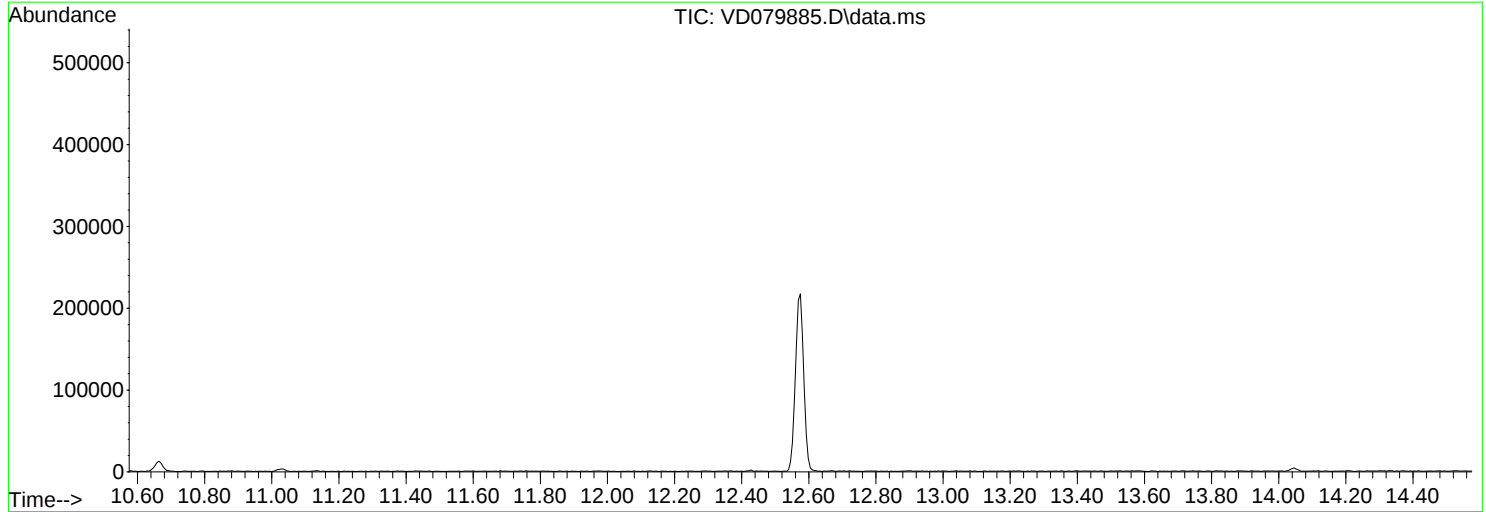

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7538	PASS
75	95	30	80	51.4	18984	PASS
95	95	100	100	100.0	36907	PASS
96	95	5	9	6.6	2432	PASS
173	174	0.00	2	1.7	505	PASS
174	95	50	120	82.0	30267	PASS
175	174	5	9	8.2	2484	PASS
176	174	95	105	95.8	28984	PASS
177	176	5	10	6.8	1957	PASS

Scan 1860 (12.528 min): VD079885.D\data.ms
BFB833

m/z	Abundance
40.10	565.0
44.00	186.0
49.90	151.0

Instrument :
MSVOA_D
ClientSampleId :
BFB833

m/z	Abundance
35.90	444.0
37.00	2382.0
38.00	2155.0
39.00	878.0
39.90	739.0
44.10	396.0
44.90	343.0
47.10	566.0
47.70	310.0
49.00	1499.0
50.00	8617.0
51.10	2898.0
54.90	155.0
55.90	1000.0
57.10	1549.0
58.20	150.0
59.80	450.0
60.00	443.0
61.00	1990.0
62.10	2394.0
63.00	2252.0
63.80	330.0
67.20	198.0
68.10	4303.0
69.00	3959.0
69.90	501.0
72.00	403.0
73.00	2203.0
74.00	6926.0
75.00	20824.0
76.00	1998.0
76.80	242.0
77.80	230.0
78.90	2606.0
79.80	729.0
80.90	2785.0
82.00	696.0
86.90	2125.0
88.10	1806.0
90.80	318.0
92.00	1485.0
92.90	2197.0
94.00	5254.0
95.10	38672.0
96.00	2558.0
103.90	497.0
105.90	281.0
114.70	168.0
116.80	654.0
117.70	312.0
119.00	282.0
127.70	211.0
128.80	171.0
129.90	167.0
136.90	230.0
140.90	881.0
143.00	1324.0
144.80	525.0
170.10	153.0
170.90	165.0
171.90	255.0
172.90	614.0
174.00	32040.0
175.00	2467.0
176.00	30080.0
177.00	1839.0
192.80	269.0
281.20	908.0
281.90	184.0

Instrument :
MSVOA_D
ClientSampleId :
BFB833

m/z	Abundance
35.90	410.0
37.00	1897.0
38.00	2136.0
39.20	490.0
40.10	453.0
43.90	701.0
44.90	407.0
47.10	383.0
48.00	469.0
49.00	1751.0
50.00	8106.0
51.00	3053.0
55.00	198.0
56.00	1142.0
57.00	1427.0
58.20	186.0
60.00	531.0
61.00	2760.0
62.10	2792.0
63.00	2042.0
63.90	312.0
64.90	213.0
68.00	3797.0
69.00	4688.0
69.90	532.0
71.90	395.0
73.00	2431.0
74.00	8017.0
75.00	20592.0
76.00	1560.0
76.80	382.0
79.00	3273.0
79.90	542.0
80.90	3525.0
81.90	720.0
86.90	2016.0
88.00	2281.0
91.00	415.0
92.00	1570.0
93.00	1625.0
93.90	4571.0
95.00	40264.0
96.10	3067.0
104.10	306.0
105.70	248.0
110.90	155.0
116.00	183.0
116.90	501.0
118.00	346.0
118.90	248.0
127.60	152.0
128.80	210.0
130.00	181.0
130.90	185.0
133.00	282.0
134.80	197.0
136.70	231.0
140.90	799.0
143.00	1270.0
144.80	499.0
154.70	207.0
170.70	167.0
172.20	355.0
173.00	902.0
174.00	32440.0
175.00	2938.0
176.00	31744.0
176.90	2076.0
191.10	247.0
193.00	268.0
206.90	188.0
281.10	1320.0
282.00	558.0
283.00	167.0

Instrument :
MSVOA_D
ClientSampleId :
BFB833

m/z	Abundance
35.90	289.0
37.00	2003.0
38.00	1683.0
39.00	520.0
40.00	594.0
44.00	573.0
44.80	246.0
45.90	171.0
47.00	351.0
47.90	244.0
48.90	1448.0
50.00	6345.0
51.00	1789.0
55.00	190.0
55.90	562.0
56.90	1028.0
60.00	371.0
61.00	1561.0
62.00	1856.0
63.00	1533.0
64.00	564.0
68.00	3578.0
69.00	3249.0
70.00	330.0
71.80	333.0
73.00	1579.0
74.00	6626.0
75.00	15537.0
76.00	1458.0
77.00	349.0
78.10	196.0
78.90	2426.0
80.10	478.0
80.90	2456.0
81.90	449.0
87.00	1173.0
87.90	1431.0
90.70	357.0
92.00	1142.0
93.00	1685.0
94.00	4340.0
95.00	31784.0
96.00	1672.0
104.00	312.0
105.80	268.0
115.70	209.0
116.90	414.0
117.90	189.0
119.00	327.0
127.70	166.0
130.10	249.0
140.80	654.0
142.80	863.0
144.60	200.0
145.00	285.0
170.60	169.0
170.90	156.0
171.50	261.0
172.20	305.0
174.00	26320.0
175.00	2048.0
176.00	25128.0
177.00	1956.0
190.90	174.0
193.00	353.0
265.00	182.0
281.20	1272.0
282.00	298.0
282.40	261.0

Instrument :
MSVOA_D
ClientSampleId :
BFB833