




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092624\
Data File : VD079908.D
Acq On : 26 Sep 2024 15:11
Operator : RP/MD
Sample : P4162-19
Misc : 5.27G/10ml/MSVOA_D/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4EJ4

Manual IntegrationsAPPROVED

Quant Time: Sep 27 01:40:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 01:31:41 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/27/2024
Supervised By :Semsettin Yesilyurt 09/27/2024

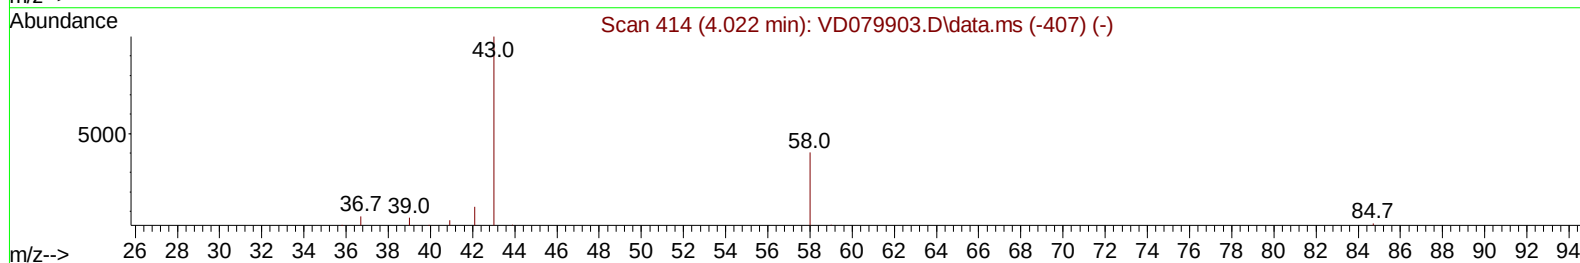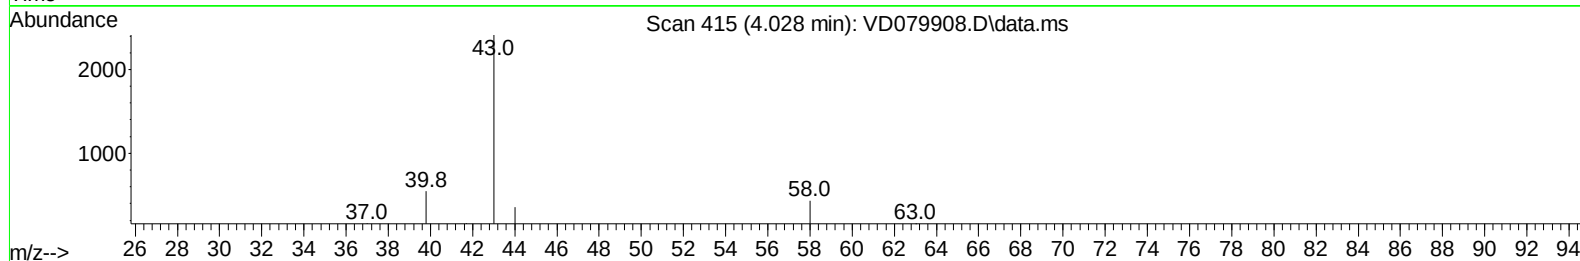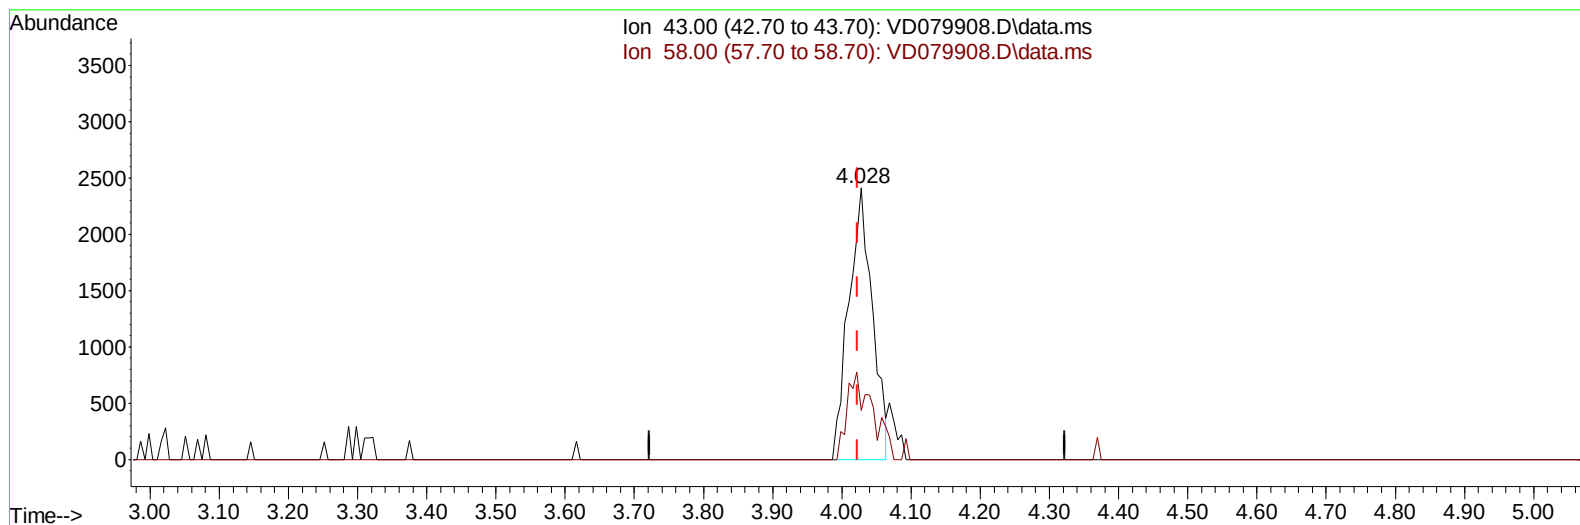

TIC: VD079908.D\data.ms

(13) Acetone (T)

4.028min (+ 0.005) 5.00 ug/L

response 5685

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.90	11.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092624\
Data File : VD079908.D
Acq On : 26 Sep 2024 15:11
Operator : RP/MD
Sample : P4162-19
Misc : 5.27G/10ml/MSVOA_D/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4EJ4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/27/2024
Supervised By :Semsettin Yesilyurt 09/27/2024

Quant Time: Sep 27 01:40:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 01:31:41 2024
Response via : Initial Calibration

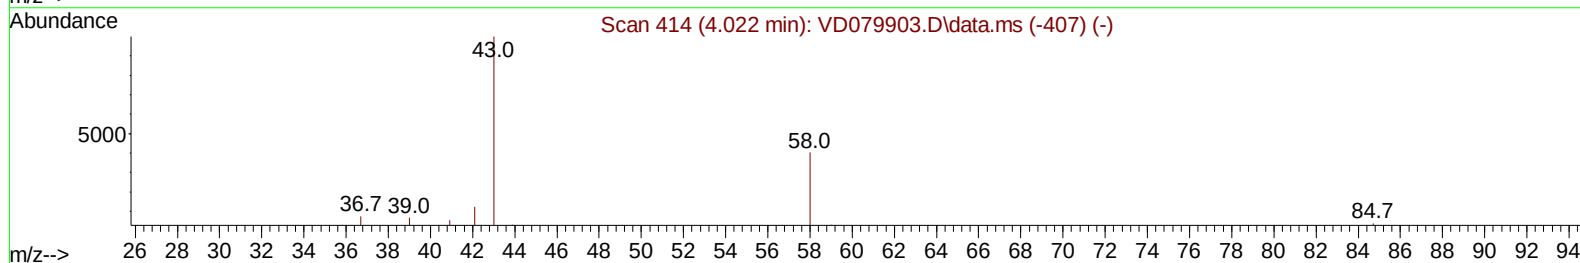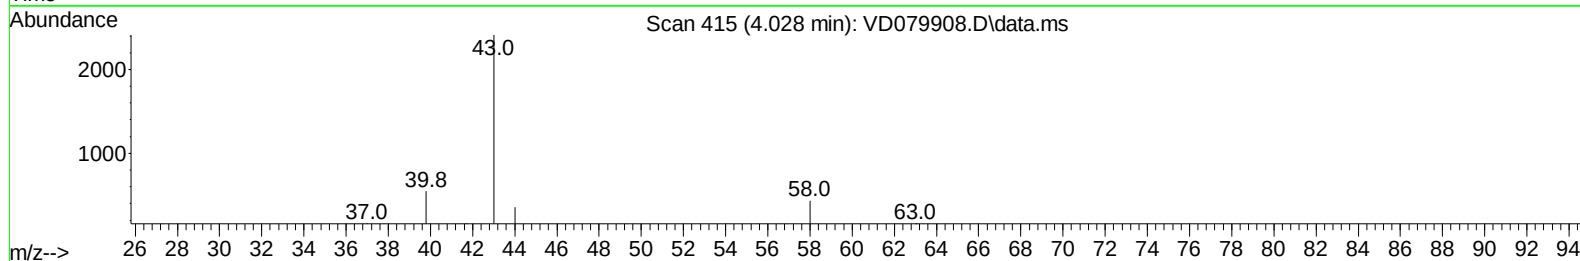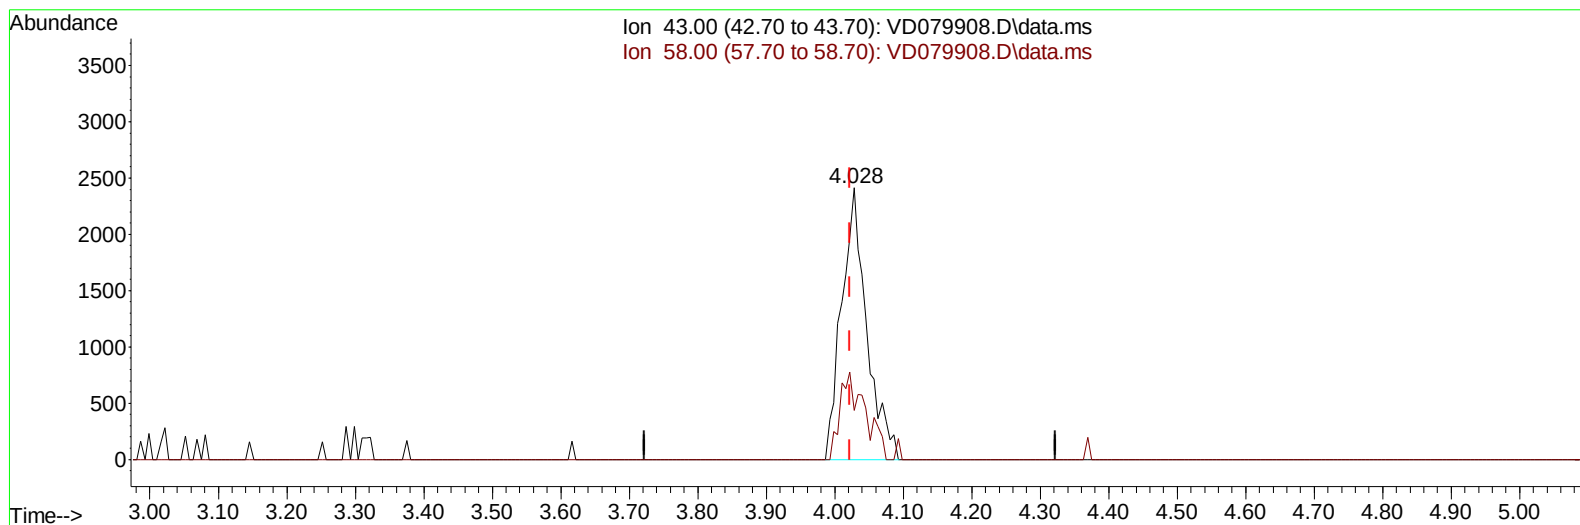

TIC: VD079908.D\data.ms

(13) Acetone (T)

4.028min (+ 0.005) 5.39 ug/L m

response 6121

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	37.90	10.24
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092624\
 Data File : VD079908.D
 Acq On : 26 Sep 2024 15:11
 Operator : RP/MD
 Sample : P4162-19
 Misc : 5.27G/10mL/MSVOA_D/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4EJ4

Manual IntegrationsAPPROVED

Quant Time: Sep 27 01:40:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 27 01:31:41 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/27/2024
 Supervised By :Semsettin Yesilyurt 09/27/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		230716	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.580	117		161077	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		32918	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		150511	15.003	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	60.000%	
7) Chloroethane-d5	2.804	69		154090	19.400	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	77.600%	
11) 1,1-Dichloroethene-d2	3.922	65		28128	15.442	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	61.760%	
21) 2-Butanone-d5	6.987	46		26944	28.906	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	57.820%	
24) Chloroform-d	7.569	84		134983	17.798	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	71.200%	
26) 1,2-Dichloroethane-d4	8.228	65		71674	18.073	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	72.280%	
32) Benzene-d6	8.204	84		274056	24.099	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	96.400%	
36) 1,2-Dichloropropane-d6	9.210	67		89584	25.721	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	102.880%	
41) Toluene-d8	10.269	98		208569	20.843	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	83.360%	
43) trans-1,3-Dichloroprop...	10.522	79		30673	20.484	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	81.920%	
47) 2-Hexanone-d5	10.875	63		22451	39.544	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	79.080%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		43260	16.903	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	67.600%	
66) 1,2-Dichlorobenzene-d4	13.810	152		24728	19.919	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	79.680%	
Target Compounds							
13) Acetone	4.028	43		6121m	5.386	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092624\
Data File : VD079908.D
Acq On : 26 Sep 2024 15:11
Operator : RP/MD
Sample : P4162-19
Misc : 5.27G/10ml/MSVOA_D/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4EJ4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/27/2024
Supervised By :Semsettin Yesilyurt 09/27/2024

Quant Time: Sep 27 01:40:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 01:31:41 2024
Response via : Initial Calibration

