
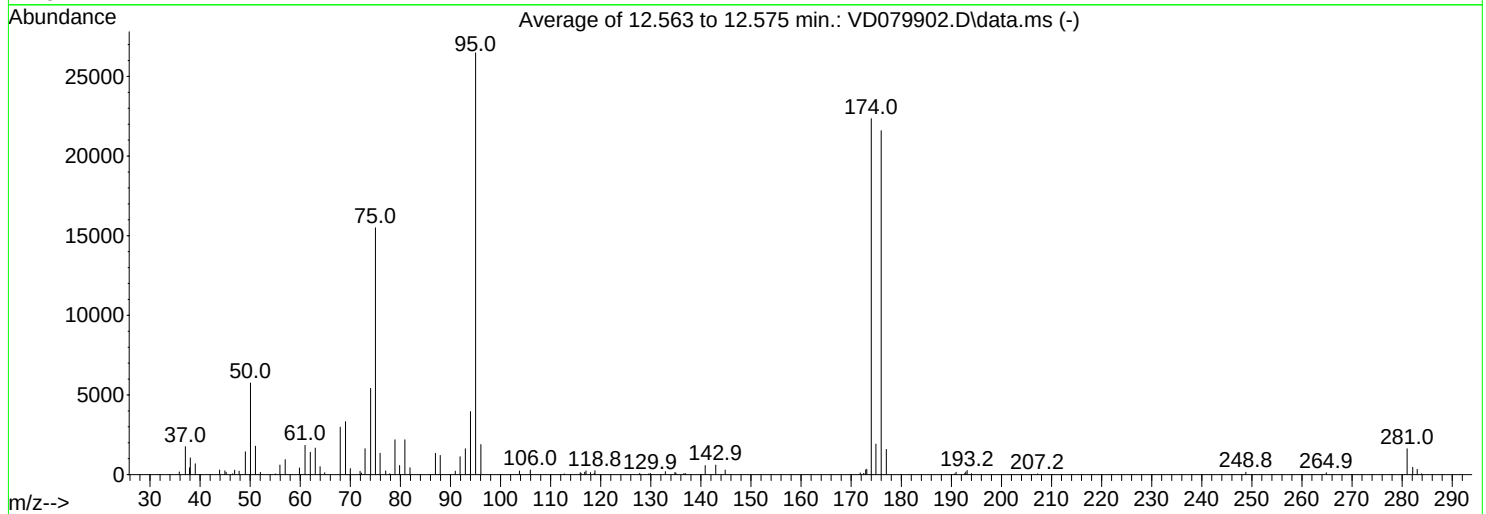


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092624\
Data File : VD079902.D
Acq On : 26 Sep 2024 11:10
Operator : RP/MD
Sample : BFB834
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB834

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Fri Sep 27 01:31:41 2024

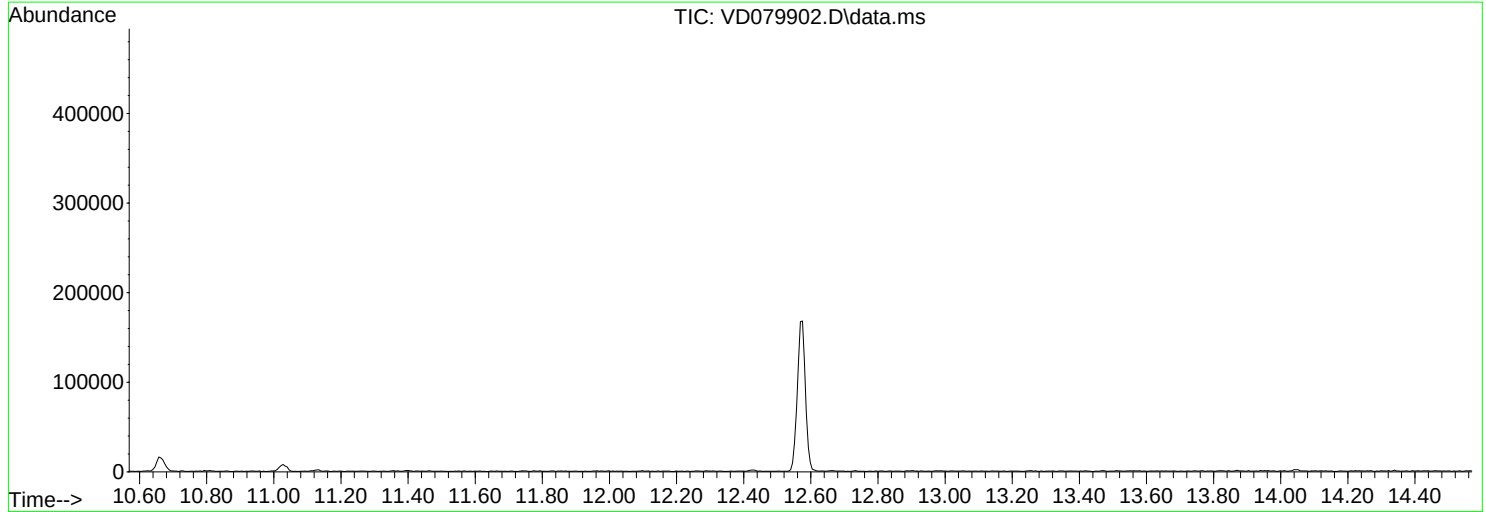

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	5761	PASS
75	95	30	80	58.5	15497	PASS
95	95	100	100	100.0	26480	PASS
96	95	5	9	7.1	1891	PASS
173	174	0.00	2	1.5	340	PASS
174	95	50	120	84.4	22355	PASS
175	174	5	9	8.6	1916	PASS
176	174	95	105	96.6	21600	PASS
177	176	5	10	7.4	1589	PASS

m/z	Abundance
40.00	391.0
43.90	220.0
98.60	156.0

Instrument :
MSVOA_D
ClientSampleId :
BFB834

m/z	Abundance
37.00	1391.0
37.90	1306.0
39.00	596.0
40.00	540.0
43.90	878.0
45.00	265.0
46.50	151.0
47.00	283.0
47.80	188.0
49.00	1135.0
50.10	5343.0
51.10	1378.0
55.00	163.0
56.00	474.0
56.90	869.0
59.90	506.0
60.90	1466.0
62.00	1277.0
63.00	1335.0
63.90	370.0
64.90	191.0
68.00	2085.0
69.10	2139.0
69.90	371.0
72.00	256.0
72.90	1790.0
74.10	4104.0
75.00	12267.0
75.90	1216.0
77.10	281.0
78.90	2001.0
79.90	480.0
80.90	1676.0
81.90	316.0
87.00	1030.0
87.90	1242.0
90.90	159.0
91.90	550.0
93.00	1346.0
94.00	3054.0
95.00	22400.0
96.10	1572.0
103.70	217.0
106.00	186.0
115.90	174.0
117.10	357.0
118.00	177.0
118.70	249.0
134.80	215.0
140.90	445.0
142.90	504.0
144.90	362.0
172.50	245.0
173.00	352.0
174.00	16880.0
174.90	1588.0
176.00	17080.0
177.00	973.0
191.00	198.0
193.10	350.0
264.80	173.0
281.00	754.0
282.10	281.0
283.10	175.0

Instrument :
MSVOA_D
ClientSampleId :
BFB834

m/z	Abundance
35.90	304.0
37.00	2094.0
38.10	1645.0
39.00	592.0
40.10	355.0
44.00	368.0
45.20	421.0
46.90	339.0
47.90	247.0
49.00	1990.0
50.00	6471.0
51.00	2072.0
52.10	203.0
56.00	820.0
57.00	1154.0
59.80	355.0
60.90	2299.0
62.10	1528.0
63.00	1753.0
64.00	414.0
68.00	3647.0
69.00	4356.0
70.00	289.0
72.20	306.0
73.00	1301.0
74.00	6290.0
75.00	16616.0
76.00	1558.0
77.00	174.0
78.90	2526.0
79.80	620.0
80.90	2152.0
81.80	644.0
87.00	1451.0
87.90	1099.0
91.00	250.0
91.90	1390.0
93.00	1754.0
94.00	4122.0
95.00	28848.0
96.00	2108.0
103.80	291.0
105.90	340.0
115.90	205.0
117.00	371.0
117.90	210.0
118.90	350.0
129.90	239.0
132.90	298.0
134.80	211.0
136.60	214.0
140.90	592.0
142.90	611.0
144.70	274.0
171.90	167.0
172.80	559.0
174.00	24840.0
174.90	1918.0
176.00	23088.0
177.00	1779.0
190.90	260.0
192.70	264.0
193.20	425.0
207.20	155.0
248.80	230.0
281.00	1919.0
282.20	496.0
283.10	257.0
283.90	159.0

Instrument :
MSVOA_D
ClientSampleId :
BFB834

m/z	Abundance
35.80	200.0
37.10	1781.0
38.00	1523.0
39.10	867.0
40.10	289.0
44.00	285.0
44.90	463.0
46.80	231.0
47.70	240.0
49.10	1185.0
50.00	5469.0
51.00	1903.0
52.00	218.0
55.90	502.0
57.10	811.0
59.90	396.0
61.00	1755.0
61.90	1420.0
63.00	1924.0
64.00	711.0
64.90	176.0
68.00	3227.0
69.00	3477.0
70.10	489.0
71.90	365.0
73.00	1791.0
74.00	5860.0
75.00	17608.0
76.00	1261.0
77.00	238.0
77.90	175.0
78.90	2037.0
79.90	611.0
80.90	2731.0
82.00	346.0
87.00	1524.0
88.00	1274.0
90.90	245.0
91.90	1437.0
92.90	1797.0
94.00	4700.0
95.00	28192.0
96.00	1993.0
103.80	186.0
106.00	352.0
112.70	155.0
116.10	214.0
116.80	456.0
118.80	400.0
127.80	241.0
129.60	155.0
132.90	291.0
135.00	311.0
136.90	224.0
140.80	692.0
143.00	708.0
144.90	235.0
171.70	159.0
173.10	1021.0
174.00	25344.0
175.00	2243.0
176.00	24632.0
177.00	2016.0
190.70	155.0
192.90	520.0
194.00	170.0
248.80	228.0
264.90	192.0
281.00	2198.0
282.00	612.0
282.90	565.0

Instrument :
MSVOA_D
ClientSampleId :
BFB834