




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
Data File : VD079919.D
Acq On : 27 Sep 2024 13:46
Operator : RP/MD
Sample : VD0927SBL01
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK823

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:01:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 23:37:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/30/2024
Supervised By :Semsettin Yesilyurt 09/30/2024

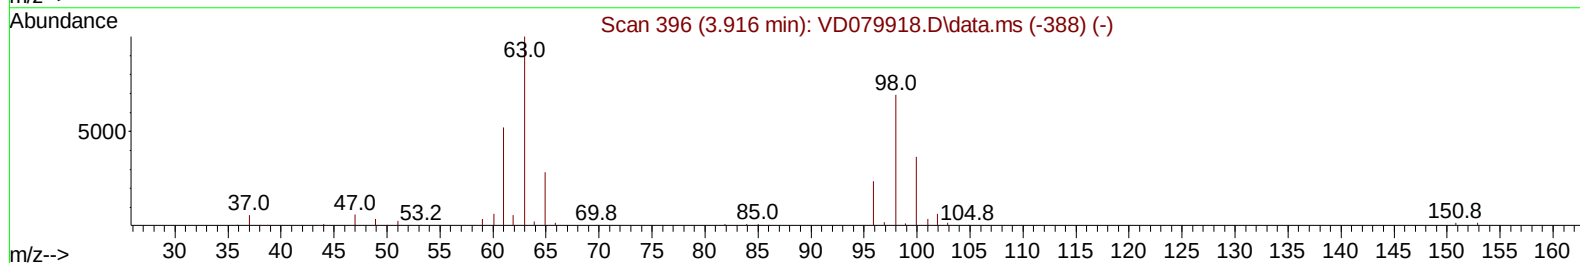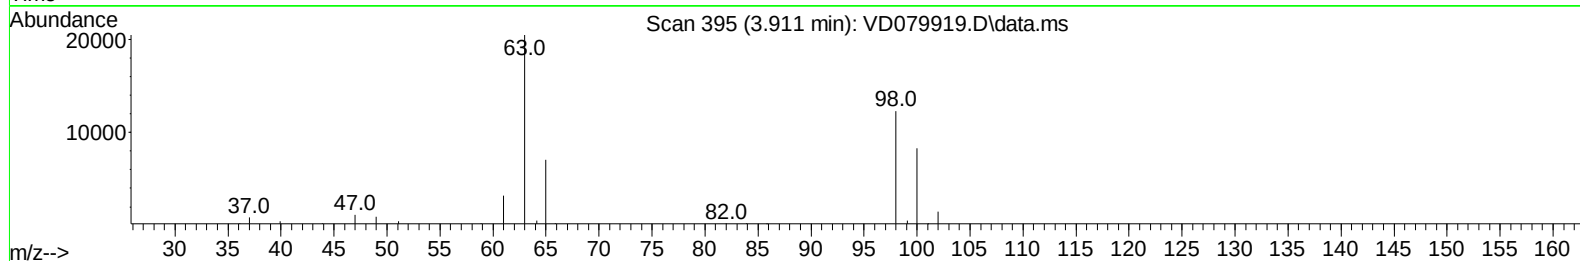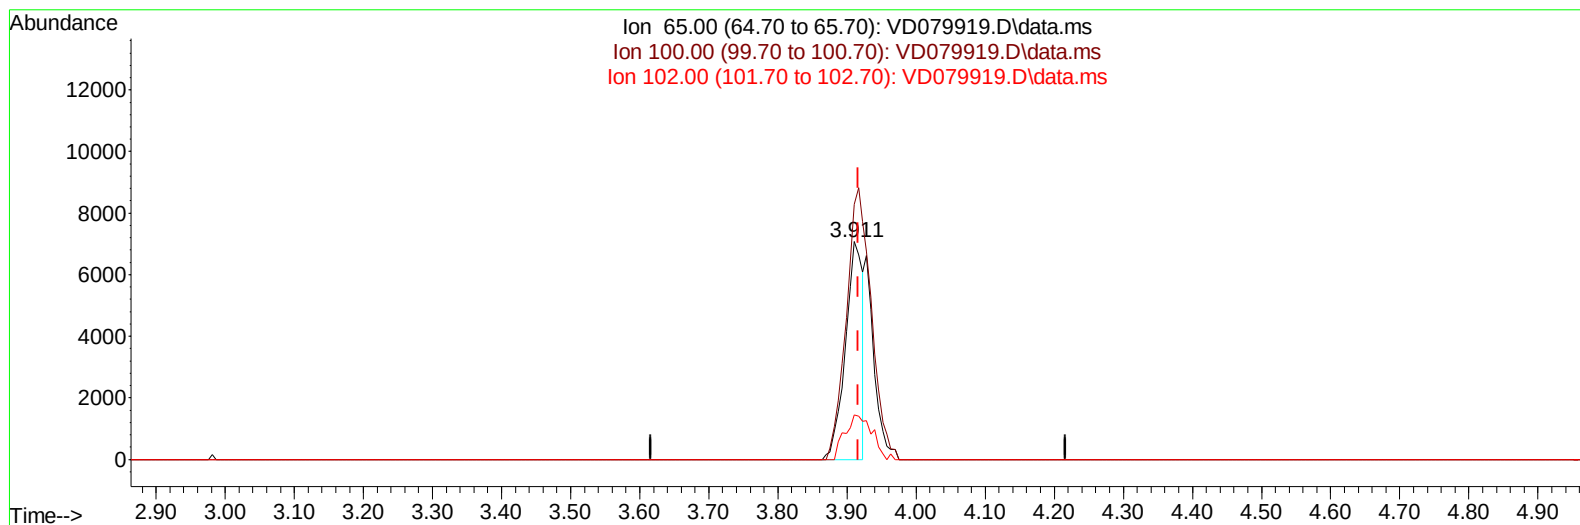

TIC: VD079919.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.911min (-0.006) 12.29 ug/L

response 12270

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	141.70	180.46
102.00	21.20	31.79#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
Data File : VD079919.D
Acq On : 27 Sep 2024 13:46
Operator : RP/MD
Sample : VD0927SBL01
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK823

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:01:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 23:37:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/30/2024
Supervised By :Semsettin Yesilyurt 09/30/2024

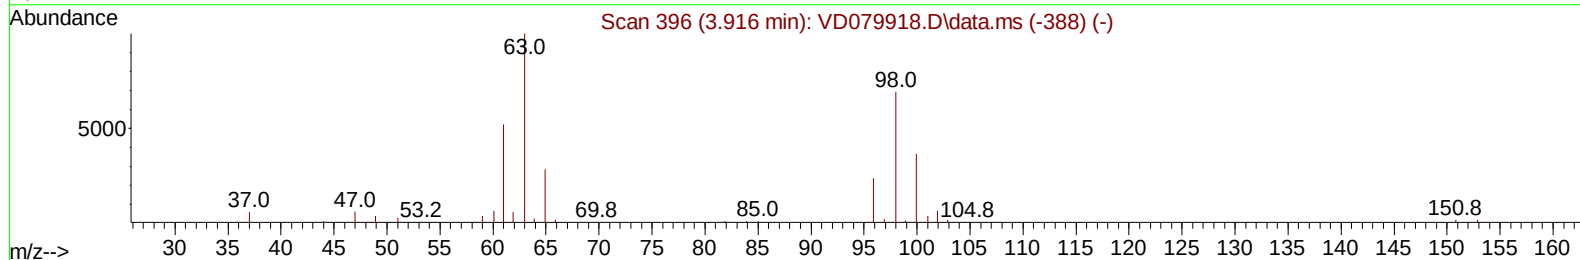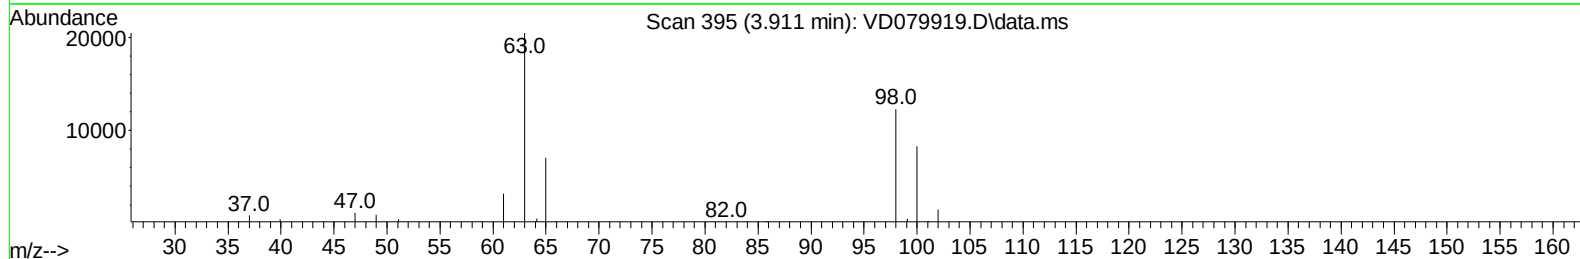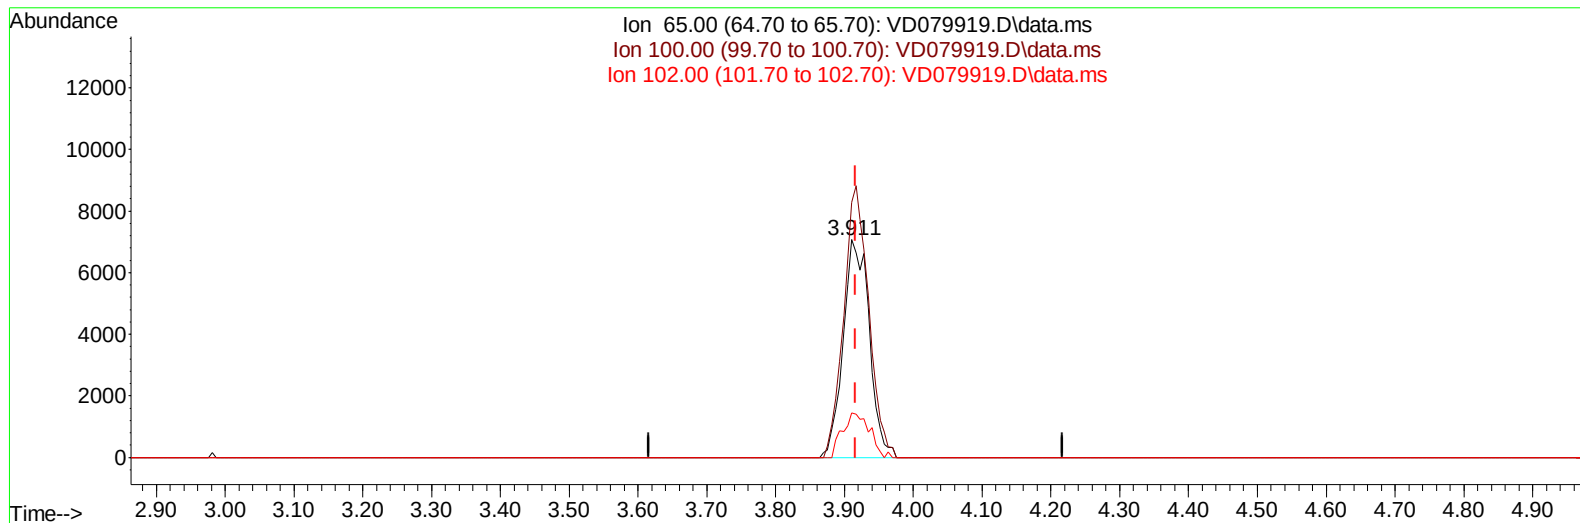

TIC: VD079919.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.911min (-0.006) 18.60 ug/L m

response 18576

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	141.70	119.20
102.00	21.20	21.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
 Data File : VD079919.D
 Acq On : 27 Sep 2024 13:46
 Operator : RP/MD
 Sample : VD0927SBL01
 Misc : 5.00G/10mL/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VBLK823

Manual IntegrationsAPPROVED

Quant Time: Sep 28 00:01:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 27 23:37:15 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/30/2024
 Supervised By :Semsettin Yesilyurt 09/30/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		126494	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		128721	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		48353	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		100764	18.319	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	73.280%	
7) Chloroethane-d5	2.799	69		102804	23.607	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	94.440%	
11) 1,1-Dichloroethene-d2	3.911	65		18576m	18.601	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	74.400%	
21) 2-Butanone-d5	6.987	46		26242	51.349	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	102.700%	
24) Chloroform-d	7.569	84		100408	24.148	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	96.600%	
26) 1,2-Dichloroethane-d4	8.228	65		55272	25.421	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	101.680%	
32) Benzene-d6	8.199	84		199198	21.920	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	87.680%	
36) 1,2-Dichloropropane-d6	9.210	67		65524	23.542	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	94.160%	
41) Toluene-d8	10.269	98		172286	21.544	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	86.160%	
43) trans-1,3-Dichloroprop...	10.528	79		26104	21.815	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	87.280%	
47) 2-Hexanone-d5	10.875	63		22106	48.723	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	97.440%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		48778	23.849	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	95.400%	
66) 1,2-Dichlorobenzene-d4	13.816	152		47336	25.959	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	103.840%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
Data File : VD079919.D
Acq On : 27 Sep 2024 13:46
Operator : RP/MD
Sample : VD0927SBL01
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VBLK823

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/30/2024
Supervised By :Semsettin Yesilyurt 09/30/2024

Quant Time: Sep 28 00:01:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 23:37:15 2024
Response via : Initial Calibration

