

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
 Data File : VD079922.D
 Acq On : 27 Sep 2024 15:07
 Operator : RP/MD
 Sample : P4162-18RE
 Misc : 5.15G/10ml/MSVOA_D/SOIL/B
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4EJ3RE

Quant Time: Sep 27 23:39:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Sep 27 23:37:15 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	141698	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	81337	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	14324	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	152302	24.718	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	98.880%	
7) Chloroethane-d5	2.805	69	152151	31.190	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	124.760%	
11) 1,1-Dichloroethene-d2	3.917	65	26252	23.467	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	93.880%	
21) 2-Butanone-d5	6.987	46	21573	37.684	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	75.360%	
24) Chloroform-d	7.569	84	133512	28.664	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	114.640%	
26) 1,2-Dichloroethane-d4	8.228	65	73654	30.240	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	120.960%	
32) Benzene-d6	8.205	84	271532	47.286	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	189.160%#	
36) 1,2-Dichloropropane-d6	9.210	67	90950	51.714	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	206.840%#	
41) Toluene-d8	10.269	98	209168	41.394	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	165.560%#	
43) trans-1,3-Dichloroprop...	10.528	79	28569	37.784	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	151.120%#	
47) 2-Hexanone-d5	10.875	63	19687	68.670	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	137.340%#	
56) 1,1,2,2-Tetrachloroeth...	12.646	84	41998	32.497	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	130.000%#	
66) 1,2-Dichlorobenzene-d4	13.816	152	22461	41.580	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	166.320%#	
Target Compounds						
25) Chloroform	7.605	83	8670	1.828	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
Data File : VD079922.D
Acq On : 27 Sep 2024 15:07
Operator : RP/MD
Sample : P4162-18RE
Misc : 5.15G/10ml/MSVOA_D/SOIL/B
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4EJ3RE

Quant Time: Sep 27 23:39:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Sep 27 23:37:15 2024
Response via : Initial Calibration

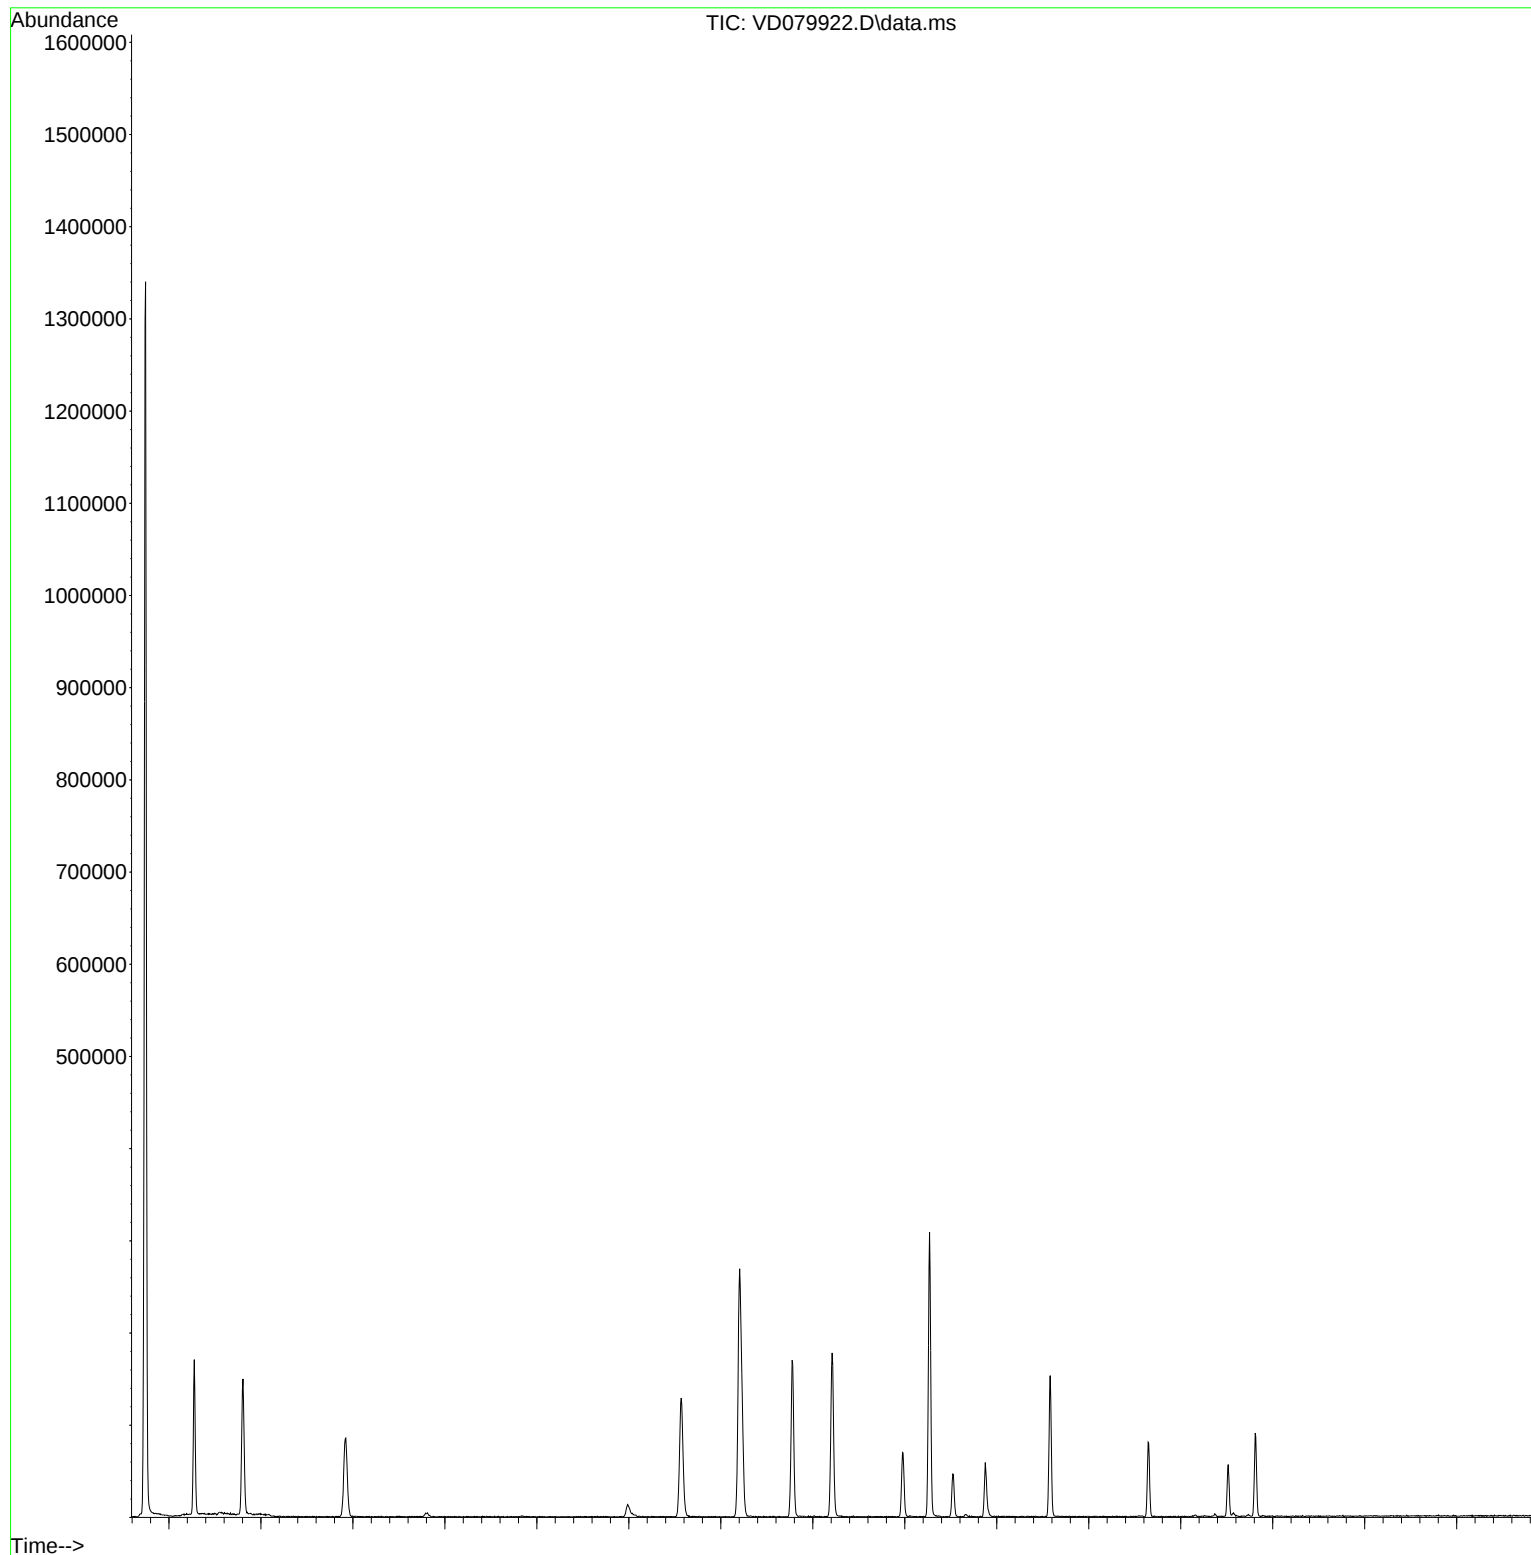

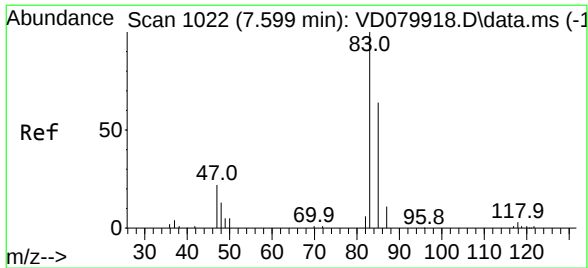

#25
Chloroform
Concen: 1.828 ug/L
RT: 7.605 min Scan# 10
Delta R.T. 0.006 min
Lab File: VD079922.D
Acq: 27 Sep 2024 15:07

Instrument :
MSVOA_D
ClientSampleId :
A4EJ3RE

Tgt Ion:	83	Resp:	8670
Ion	Ratio	Lower	Upper
83	100		
85	55.9	47.3	87.9

