
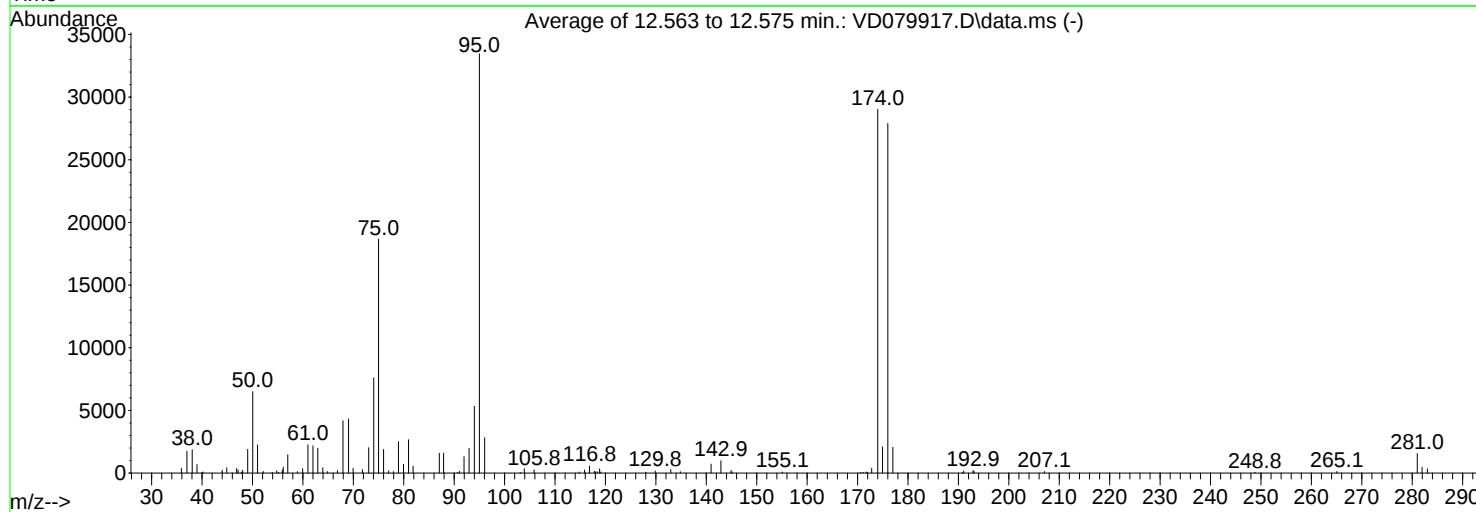


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD092724\
Data File : VD079917.D
Acq On : 27 Sep 2024 10:22
Operator : RP/MD
Sample : BFB835
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB835

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM091024SMA.M
Title : SFAM01.0
Last Update : Fri Sep 27 23:37:15 2024

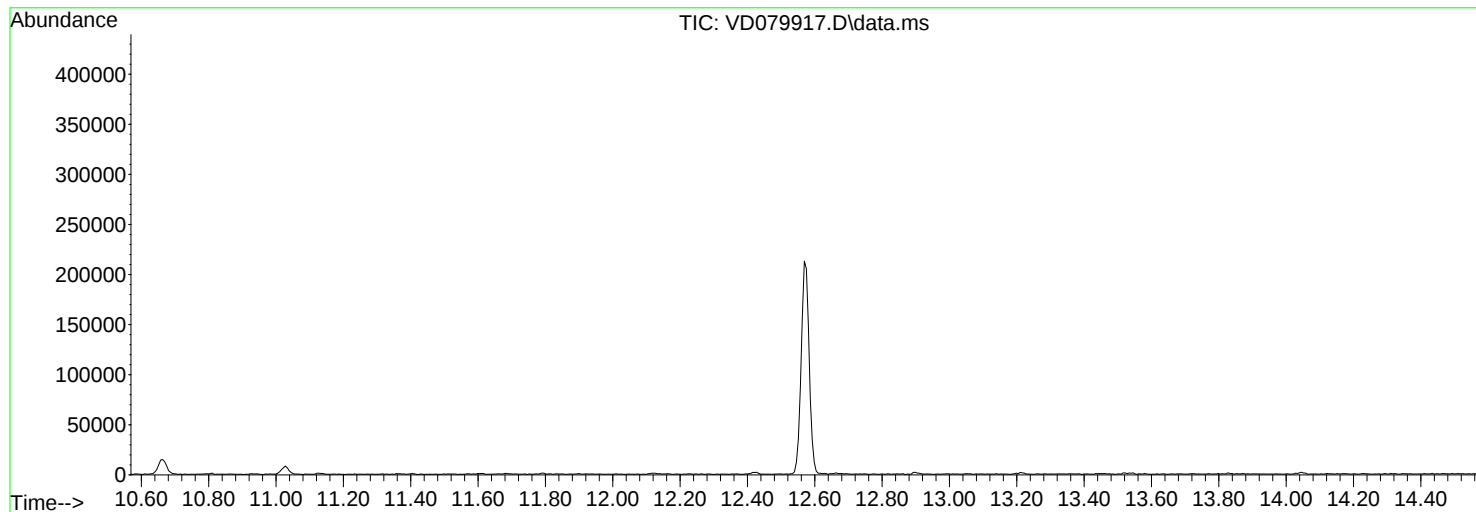

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	6494	PASS
75	95	30	80	55.8	18670	PASS
95	95	100	100	100.0	33461	PASS
96	95	5	9	8.5	2832	PASS
173	174	0.00	2	1.3	387	PASS
174	95	50	120	86.8	29032	PASS
175	174	5	9	7.2	2094	PASS
176	174	95	105	96.1	27893	PASS
177	176	5	10	7.4	2056	PASS

Scan 1859 (12.522 min): VD079917.D\data.ms
BFB835

m/z	Abundance
40.00	312.0
44.00	414.0

Instrument :
MSVOA_D
ClientSampleId :
BFB835

m/z	Abundance
35.90	485.0
37.00	1452.0
38.10	1484.0
39.00	496.0
40.00	453.0
44.00	688.0
44.90	352.0
46.80	487.0
47.20	498.0
48.20	214.0
49.00	1590.0
50.00	5592.0
51.00	1889.0
52.10	162.0
54.80	340.0
55.90	760.0
57.00	1307.0
58.90	158.0
60.00	333.0
61.00	2251.0
62.00	1998.0
63.00	1875.0
64.00	469.0
66.90	199.0
68.00	3462.0
69.10	3787.0
71.80	268.0
73.00	1662.0
74.10	6785.0
75.00	15449.0
76.00	1369.0
77.90	215.0
79.00	1873.0
79.90	630.0
81.00	2377.0
81.80	512.0
87.00	1201.0
87.80	941.0
90.70	173.0
91.90	1038.0
92.90	1782.0
94.00	4205.0
95.00	27160.0
96.00	2757.0
104.00	378.0
105.90	197.0
115.80	219.0
116.90	462.0
117.80	212.0
118.90	500.0
130.00	171.0
133.00	186.0
134.80	186.0
141.00	646.0
143.00	625.0
144.90	272.0
170.60	182.0
172.80	503.0
174.00	23424.0
175.00	1737.0
176.00	20896.0
177.00	1831.0
190.80	151.0
192.90	178.0
280.90	1132.0
282.00	382.0
283.00	270.0

Instrument :
MSVOA_D
ClientSampleId :
BFB835

m/z	Abundance
36.00	351.0
37.00	2154.0
38.00	1956.0
39.00	811.0
40.20	278.0
44.00	701.0
44.90	302.0
46.90	604.0
48.00	456.0
49.10	1889.0
50.10	7690.0
51.00	2375.0
53.90	151.0
55.20	197.0
56.10	782.0
57.00	1915.0
58.90	185.0
60.00	377.0
61.00	2572.0
62.00	2179.0
62.90	1996.0
63.90	403.0
65.00	160.0
66.70	154.0
67.90	4358.0
69.00	4705.0
69.90	439.0
71.90	382.0
73.10	2087.0
74.00	8223.0
75.00	20352.0
76.00	2190.0
77.10	281.0
78.90	2732.0
80.00	884.0
80.90	2917.0
81.90	617.0
87.10	1542.0
87.90	2212.0
91.10	277.0
92.00	1581.0
93.00	2197.0
94.00	6418.0
95.00	36992.0
96.10	2484.0
103.10	178.0
103.80	335.0
105.90	348.0
114.80	266.0
115.80	298.0
116.80	647.0
117.80	214.0
118.80	511.0
128.00	220.0
129.80	344.0
133.00	438.0
140.90	1007.0
142.80	984.0
144.90	338.0
172.00	174.0
172.80	659.0
174.00	32752.0
174.90	2263.0
176.00	31248.0
177.00	2330.0
191.10	243.0
193.10	453.0
207.10	157.0
265.10	181.0
281.00	1350.0
281.90	565.0
283.00	437.0

Instrument :
MSVOA_D
ClientSampleId :
BFB835

m/z	Abundance
35.80	309.0
37.00	1628.0
38.10	2145.0
39.00	721.0
40.00	638.0
44.00	534.0
44.90	640.0
47.10	257.0
47.80	249.0
49.00	2189.0
50.10	6199.0
51.00	2452.0
52.20	220.0
54.80	204.0
56.10	623.0
57.00	1178.0
59.90	358.0
61.00	1940.0
62.00	2349.0
63.00	2074.0
64.00	398.0
64.80	214.0
66.90	244.0
68.00	4710.0
69.00	4471.0
70.00	702.0
71.70	173.0
73.00	2339.0
74.10	7781.0
75.00	20208.0
76.00	2109.0
76.90	257.0
78.00	161.0
78.90	2949.0
79.90	586.0
80.90	2692.0
81.90	519.0
87.00	2009.0
88.00	1621.0
90.90	153.0
92.00	1310.0
93.00	1912.0
94.00	5357.0
95.00	36232.0
96.00	3254.0
103.90	353.0
105.70	238.0
115.90	196.0
116.80	591.0
118.00	330.0
118.40	319.0
119.10	251.0
132.80	220.0
134.90	164.0
140.90	514.0
142.90	1351.0
145.10	318.0
155.10	260.0
171.10	165.0
171.70	265.0
174.00	30920.0
175.00	2283.0
176.00	31536.0
177.00	2006.0
191.00	306.0
192.90	437.0
207.00	213.0
248.80	200.0
265.00	202.0
281.10	2191.0
281.90	428.0
283.00	311.0

Instrument :
MSVOA_D
ClientSampleId :
BFB835