
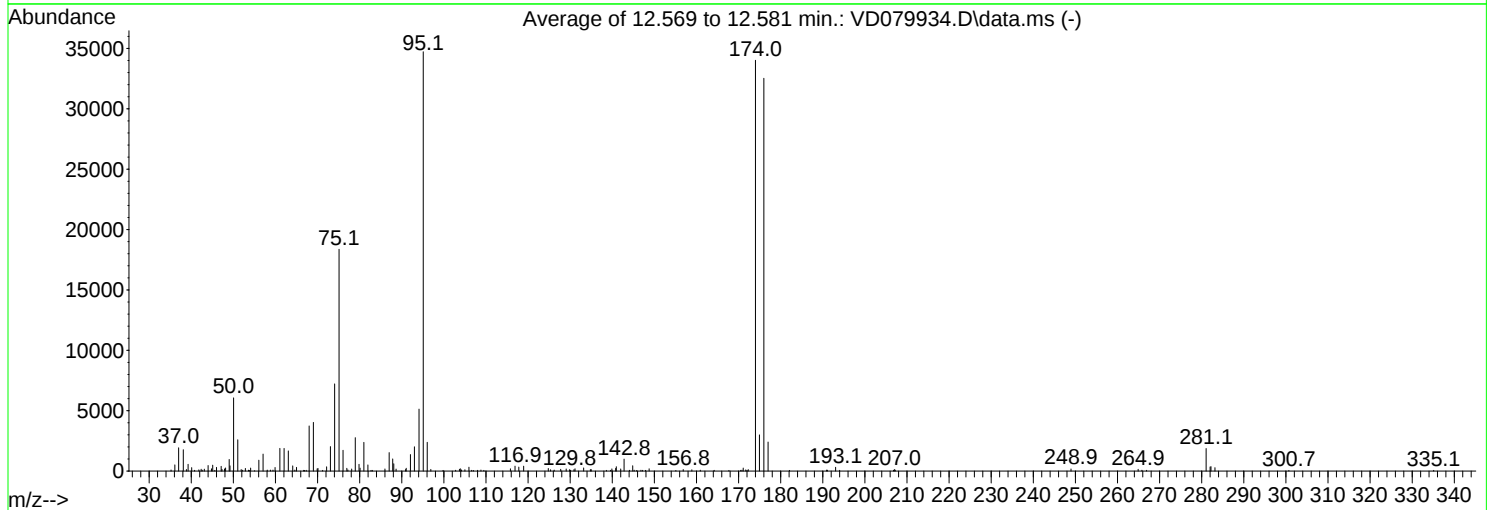


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD093024\
Data File : VD079934.D
Acq On : 30 Sep 2024 14:01
Operator : RP/MD
Sample : BFB
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D093024S.M
Title : SW846 8260
Last Update : Tue Oct 01 05:47:39 2024

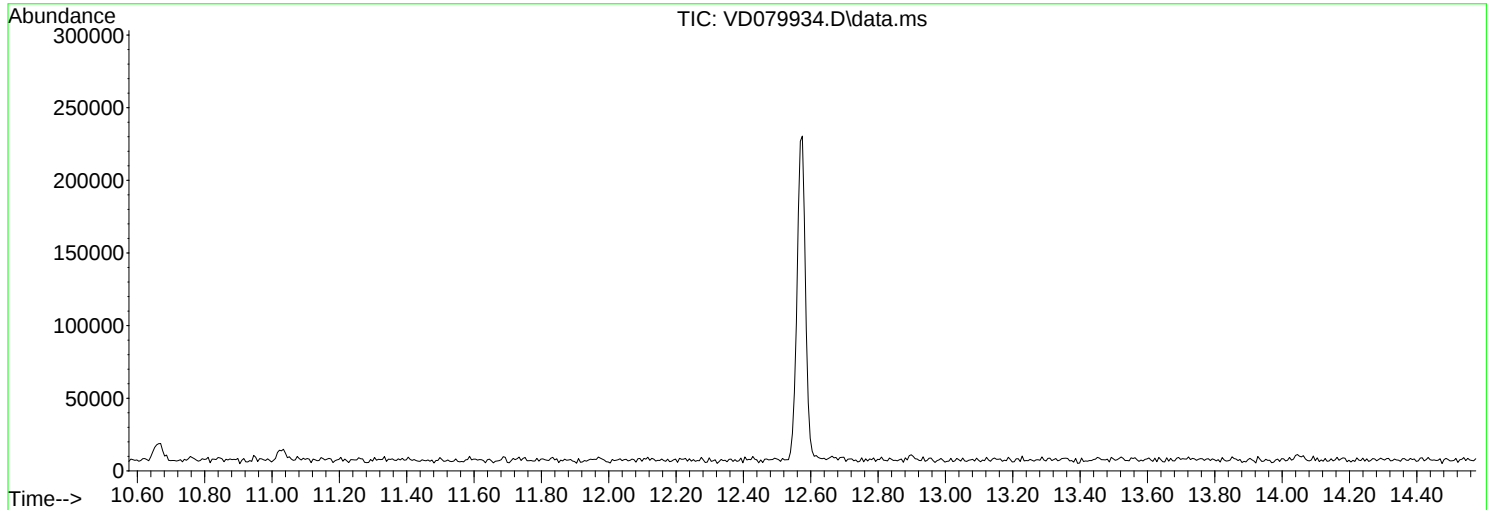

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6063	PASS
75	95	30	60	52.9	18369	PASS
95	95	100	100	100.0	34728	PASS
96	95	5	9	6.9	2383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	98.0	34019	PASS
175	174	5	9	8.8	2997	PASS
176	174	95	101	95.6	32528	PASS
177	176	5	9	7.4	2404	PASS