
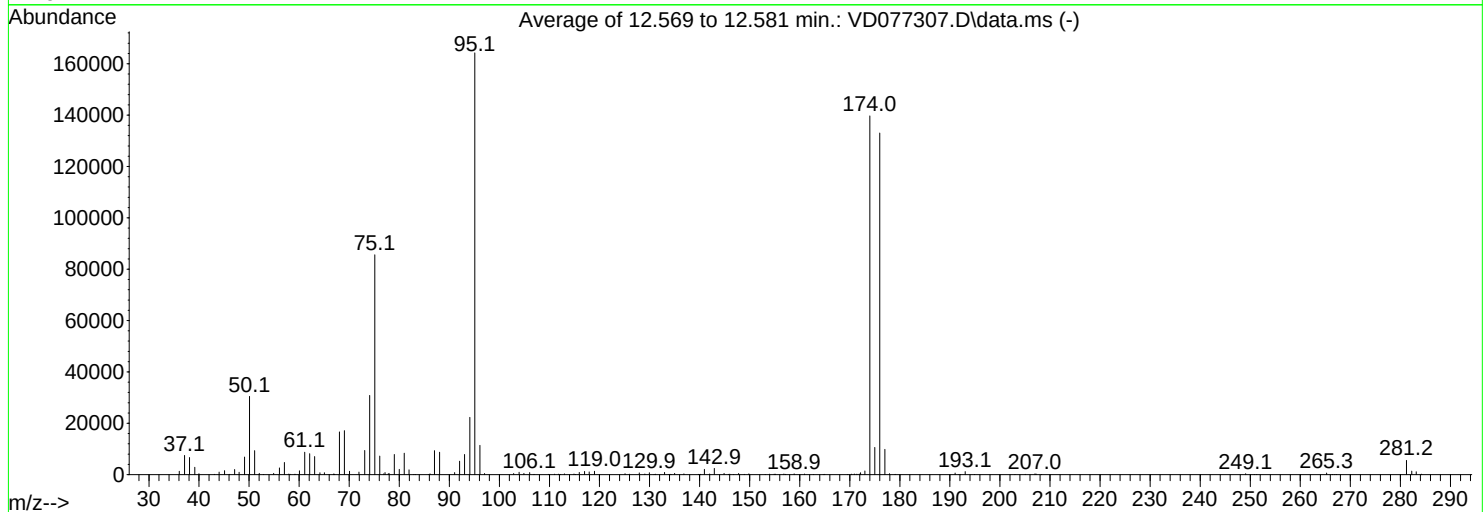


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101123\
Data File : VD077307.D
Acq On : 11 Oct 2023 15:16
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101123S.M
Title : SW846 8260
Last Update : Thu Oct 12 14:39:07 2023

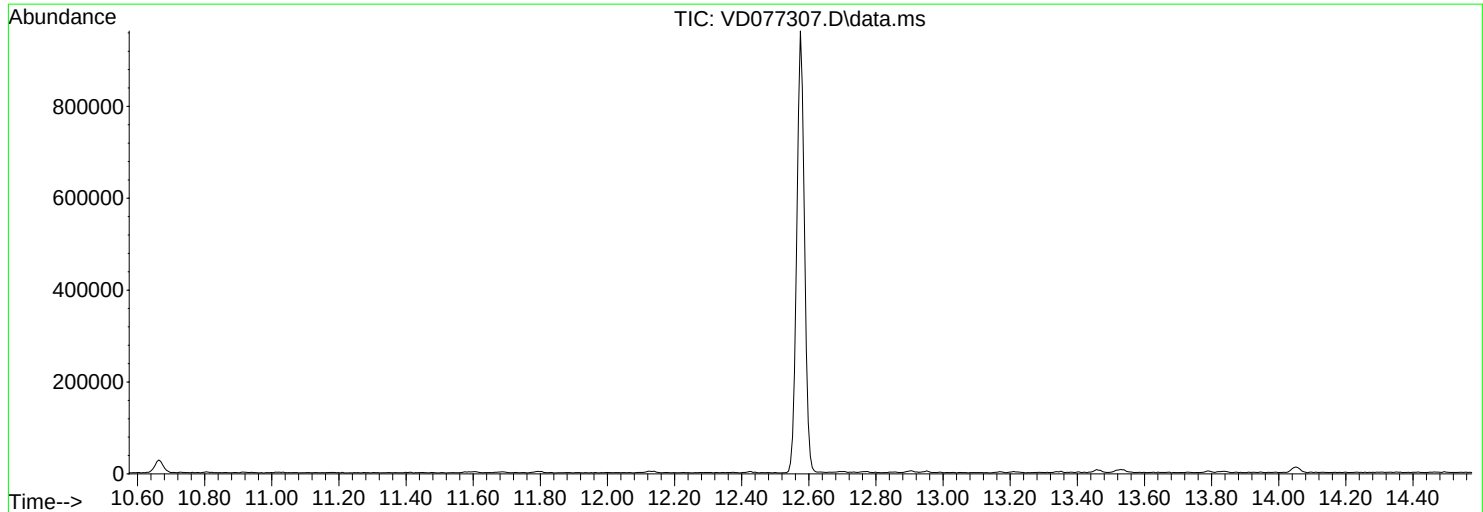

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	30456	PASS
75	95	30	60	52.1	85600	PASS
95	95	100	100	100.0	164245	PASS
96	95	5	9	6.9	11388	PASS
173	174	0.00	2	1.0	1457	PASS
174	95	50	100	85.1	139712	PASS
175	174	5	9	7.6	10576	PASS
176	174	95	101	95.2	133051	PASS
177	176	5	9	7.4	9842	PASS