
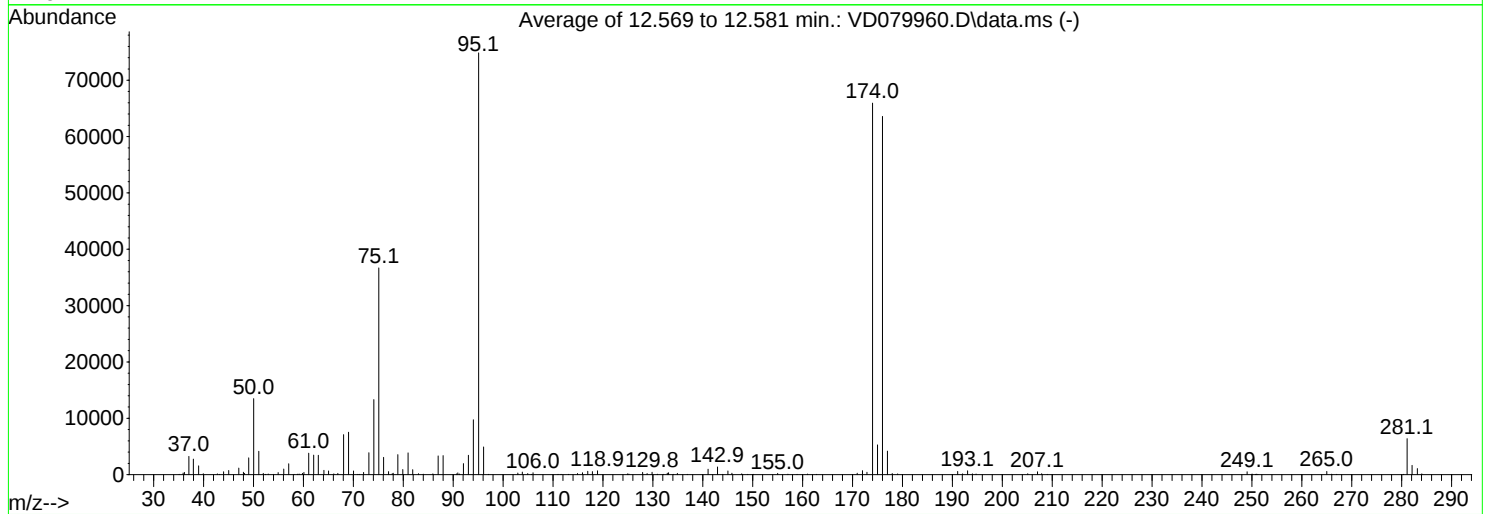


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101124\
Data File : VD079960.D
Acq On : 11 Oct 2024 09:55
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101124S.M
Title : SW846 8260
Last Update : Mon Oct 14 03:20:54 2024

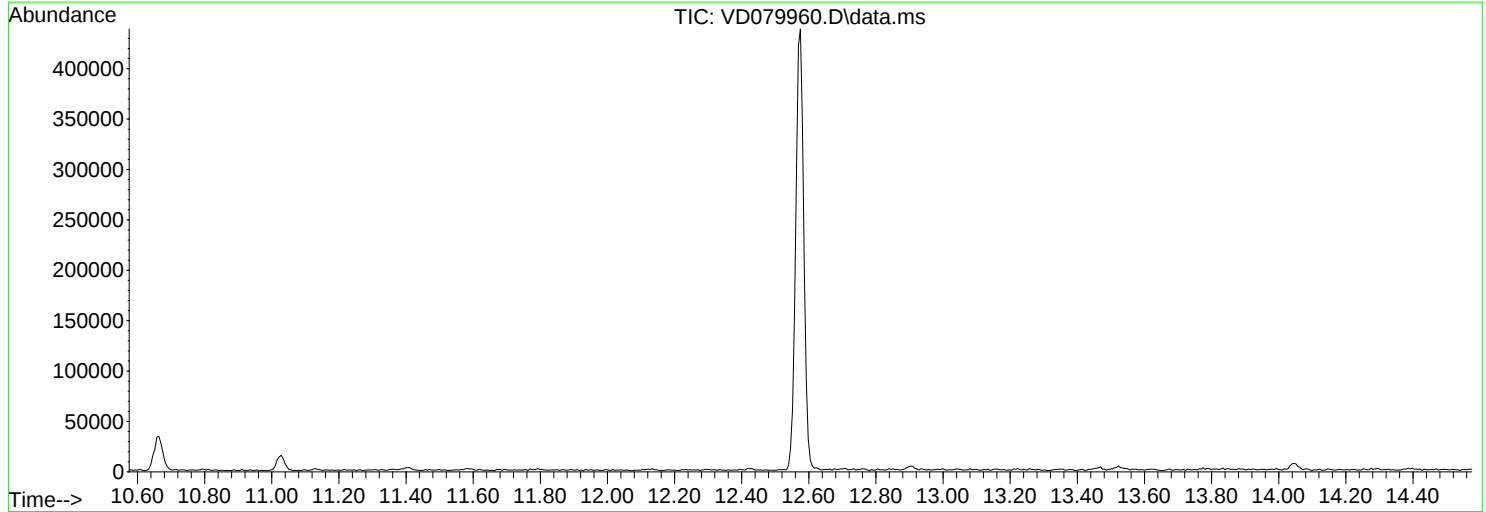


AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.0	13500	PASS
75	95	30	60	49.0	36699	PASS
95	95	100	100	100.0	74864	PASS
96	95	5	9	6.6	4910	PASS
173	174	0.00	2	0.6	419	PASS
174	95	50	100	88.1	65952	PASS
175	174	5	9	8.0	5285	PASS
176	174	95	101	96.4	63587	PASS
177	176	5	9	6.6	4187	PASS

Methylene Chloride

Response Ratio

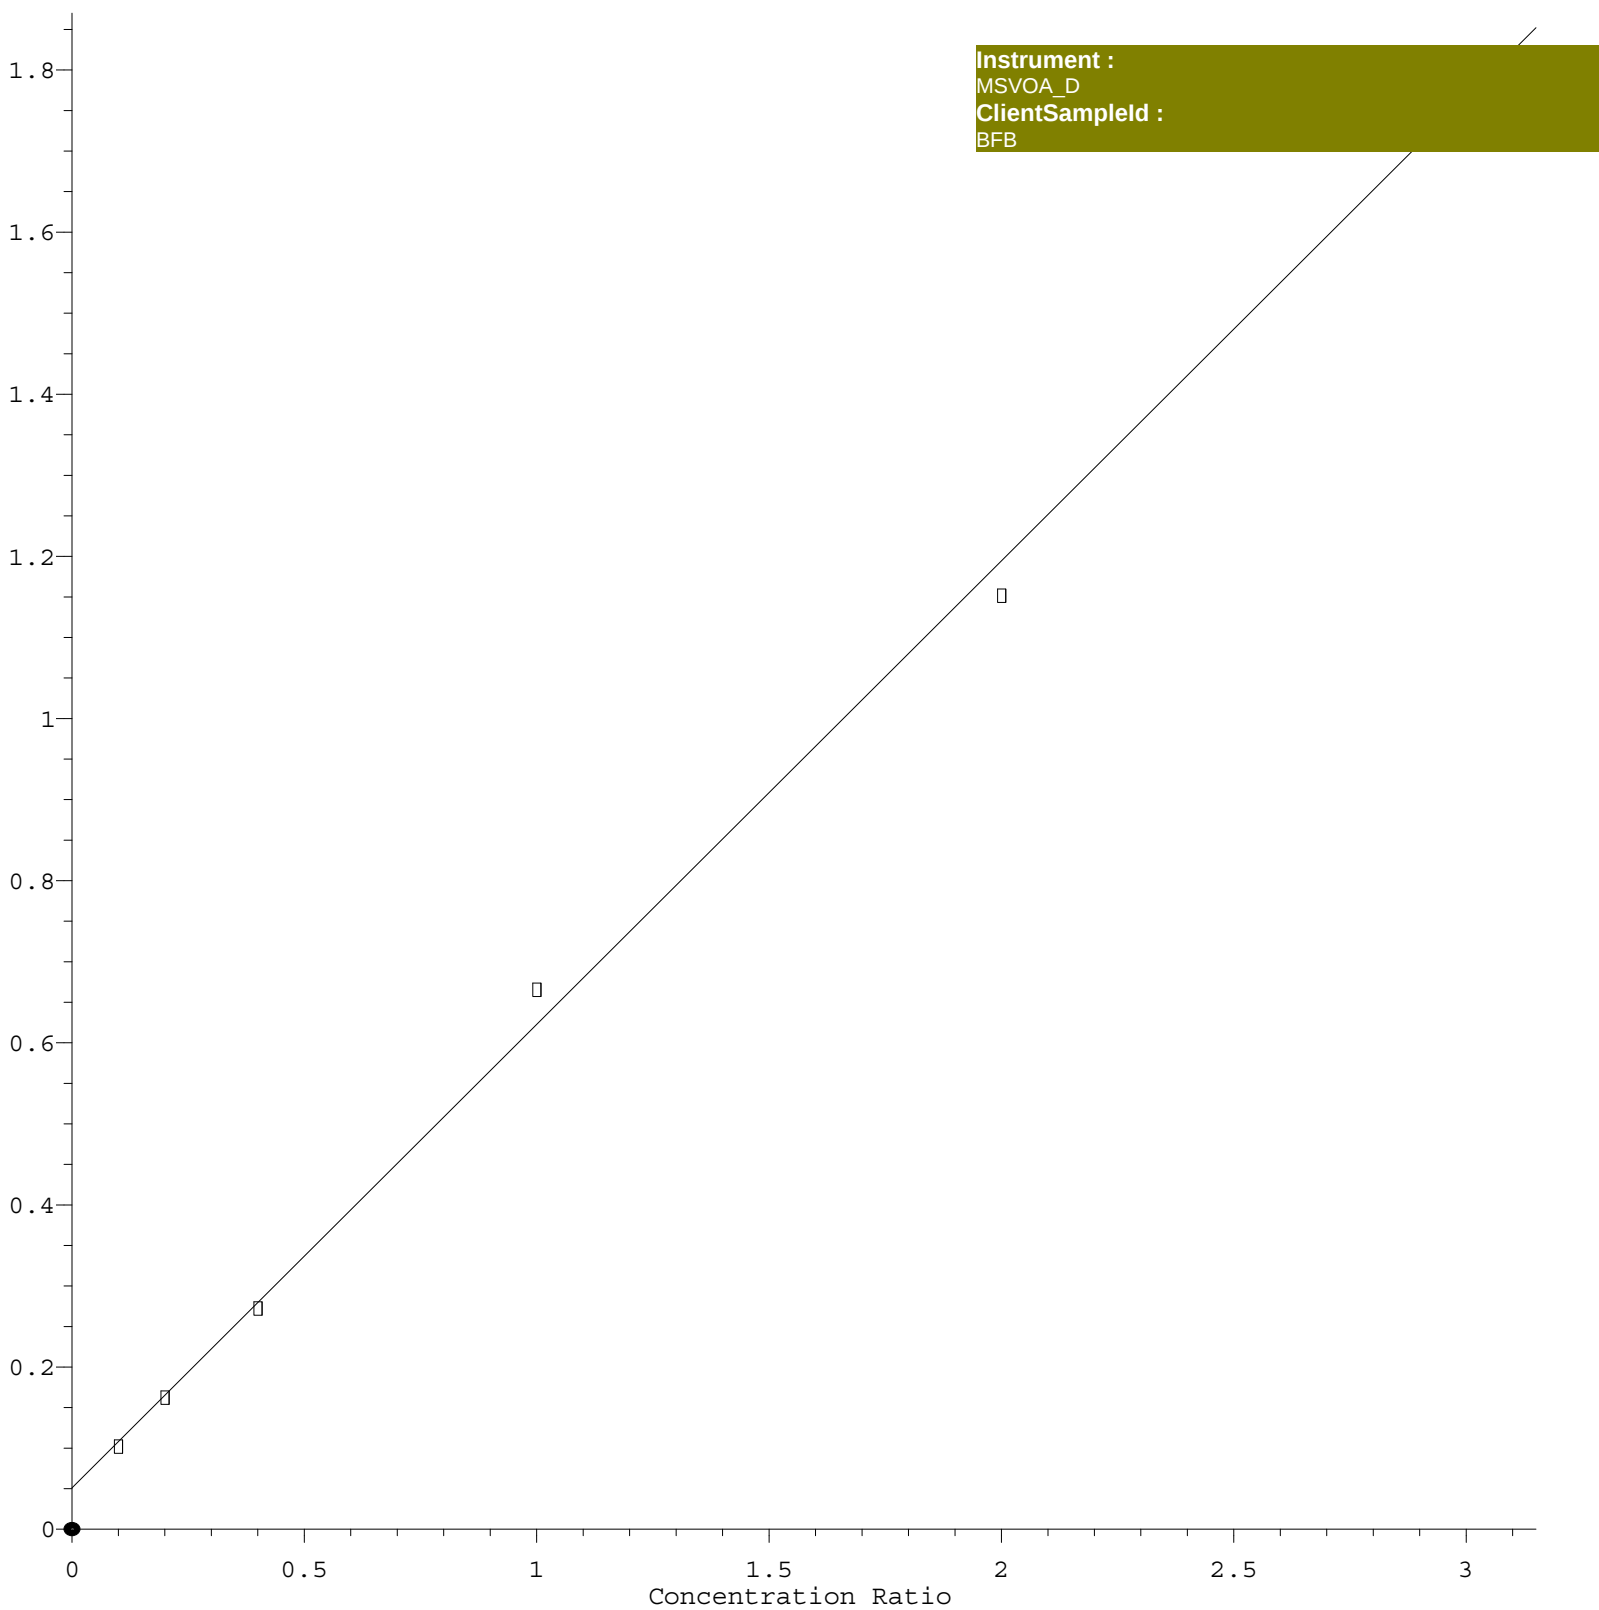

$$\text{Response} = 5.717\text{e-}001 * \text{Amt} + 5.058\text{e-}002$$

Coef of Det (r^2) = 0.998187 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D101124S.M

Calibration Table Last Updated: Mon Oct 14 03:20:54 2024