
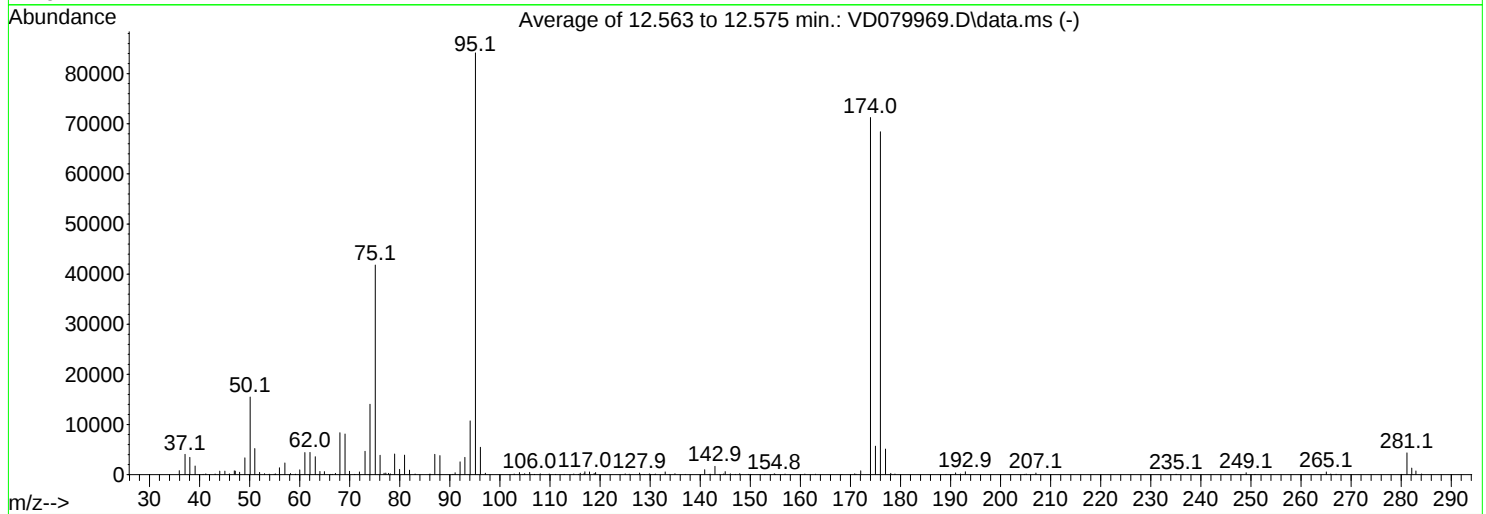


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101424\
Data File : VD079969.D
Acq On : 14 Oct 2024 08:59
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D1011245.M
Title : SW846 8260
Last Update : Mon Oct 14 03:20:54 2024

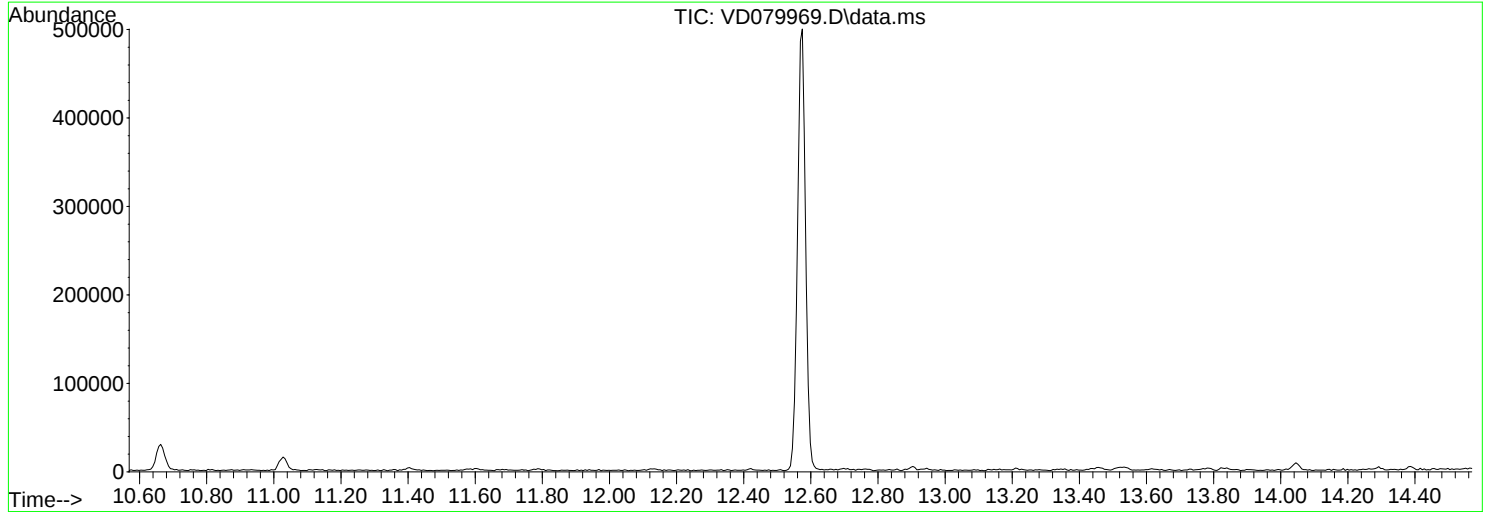

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	15484	PASS
75	95	30	60	49.7	41819	PASS
95	95	100	100	100.0	84149	PASS
96	95	5	9	6.5	5453	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.7	71243	PASS
175	174	5	9	8.0	5677	PASS
176	174	95	101	96.0	68392	PASS
177	176	5	9	7.5	5127	PASS