

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101722\
 Data File : VD074554.D
 Acq On : 17 Oct 2022 19:39
 Operator : VA/SY
 Sample : N5162-01
 Misc : 5.05G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TR-4-101422

Quant Time: Oct 17 23:10:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101122S.M
 Quant Title : SW846 8260
 QLast Update : Wed Oct 12 13:14:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.881	168	4041	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	7306	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	7953	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	3625	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.240	65	3720	106.948	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	= 213.900%#	
35) Dibromofluoromethane	7.805	113	3659	85.074	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 170.140%#	
50) Toluene-d8	10.269	98	9551	56.860	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 113.720%	
62) 4-Bromofluorobenzene	12.569	95	3190	63.585	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 127.160%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.140	50	287	5.902	ug/l	# 37
5) Bromomethane	2.693	94	87	2.438	ug/l	# 3
10) Methyl Iodide	4.175	142	56	6.031	ug/l	# 43
16) Acetone	4.022	43	73	9.729	ug/l	# 37
20) Methylene Chloride	4.805	84	397	Below Cal	#	59
36) 1,1-Dichloropropene	7.875	75	193	2.753	ug/l	# 39
38) Carbon Tetrachloride	7.875	117	209	3.224	ug/l	# 14
76) 1,2,3-Trichloropropane	12.575	75	1623	52.389	ug/l	# 1
81) trans-1,4-Dichloro-2-b...	12.575	75	1623	132.891	ug/l	# 17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD101722\
Data File : VD074554.D
Acq On : 17 Oct 2022 19:39
Operator : VA/SY
Sample : N5162-01
Misc : 5.05G/5.00ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422

Quant Time: Oct 17 23:10:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D101122S.M
Quant Title : SW846 8260
QLast Update : Wed Oct 12 13:14:00 2022
Response via : Initial Calibration




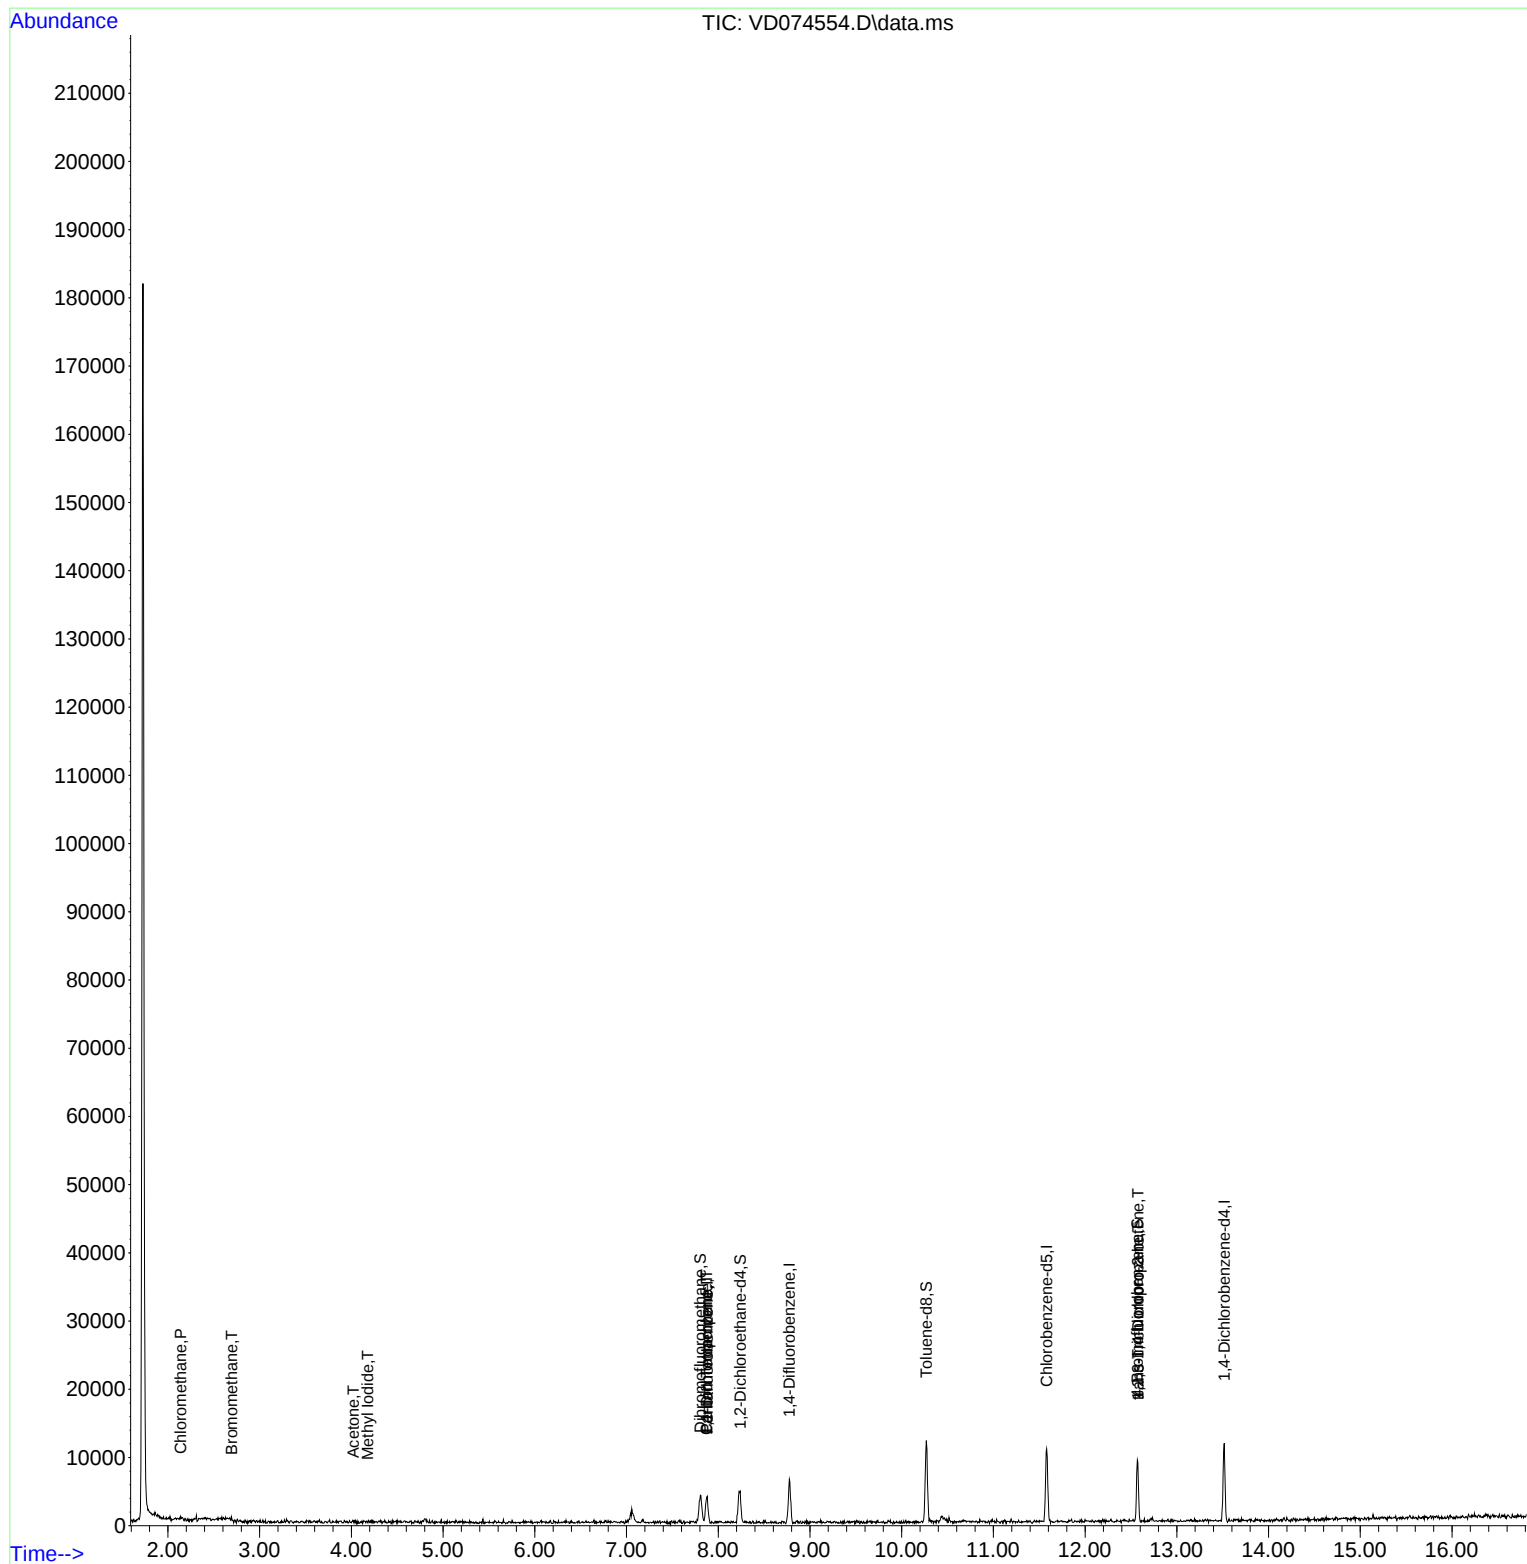


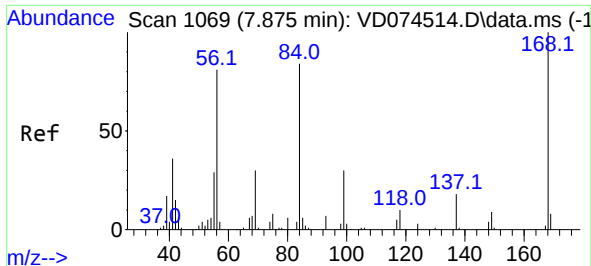

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.881 min Scan# 10
Delta R.T. 0.006 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion:168 Resp: 4041
Ion Ratio Lower Upper
168 100
99 38.9 40.9 61.3#

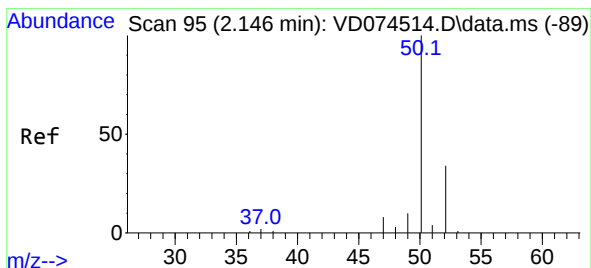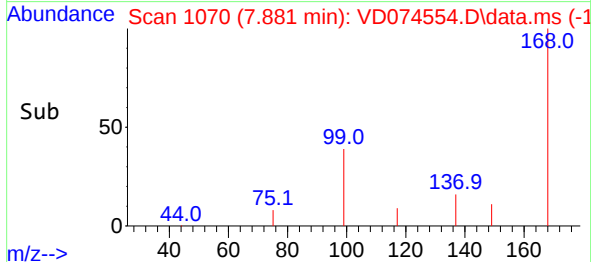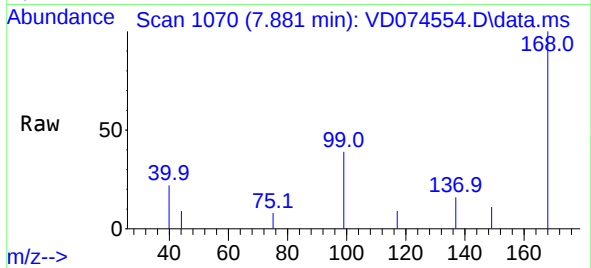

#3
Chloromethane
Concen: 5.902 ug/l
RT: 2.140 min Scan# 94
Delta R.T. 0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion: 50 Resp: 287
Ion Ratio Lower Upper
50 100
52 0.0 30.0 45.0#


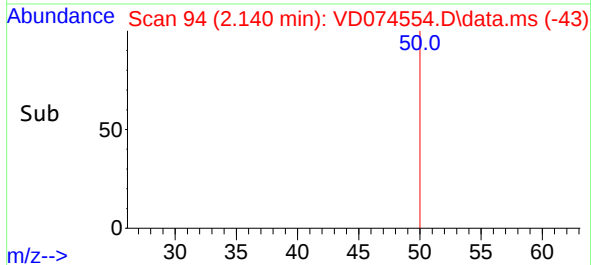

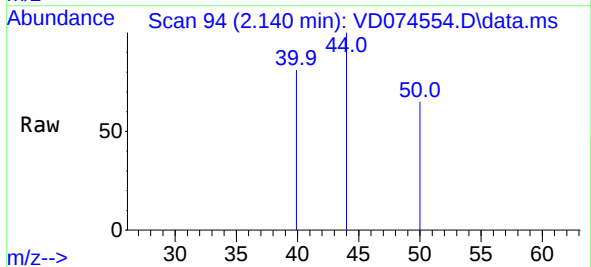


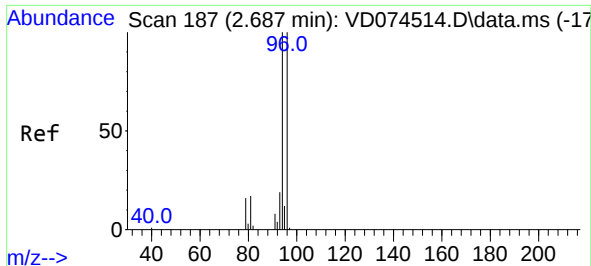

#5
Bromomethane
Concen: 2.438 ug/l
RT: 2.693 min Scan# 11
Delta R.T. 0.012 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion: 94 Resp: 87
Ion Ratio Lower Upper
94 100
96 0.0 74.6 112.0#

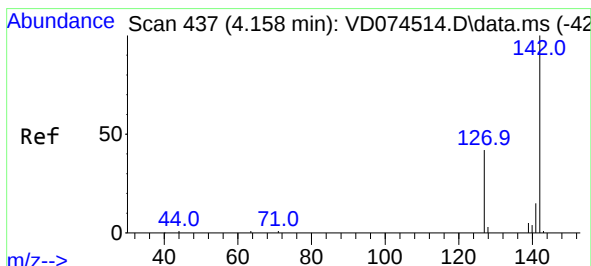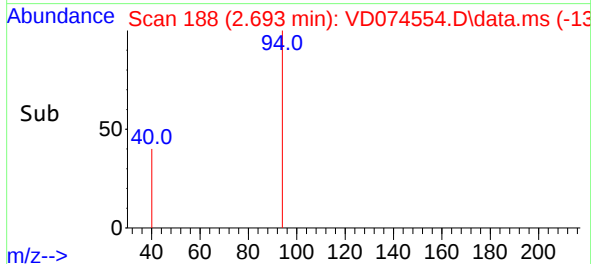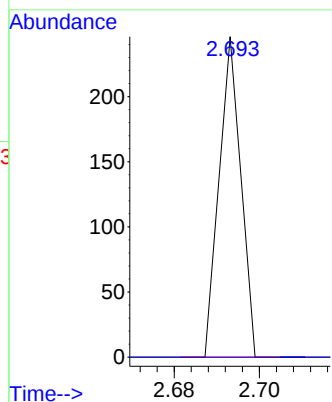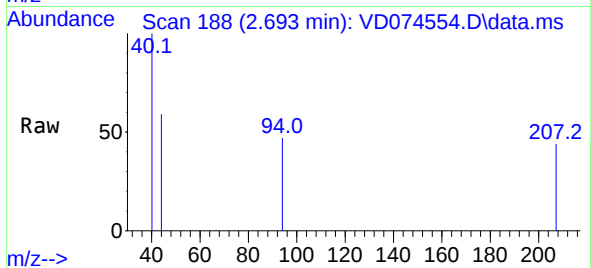

#10
Methyl Iodide
Concen: 6.031 ug/l
RT: 4.175 min Scan# 440
Delta R.T. 0.017 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion:142 Resp: 56
Ion Ratio Lower Upper
142 100
127 0.0 31.9 47.9#
141 0.0 11.4 17.2#


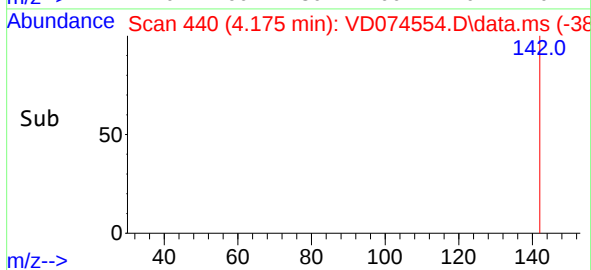

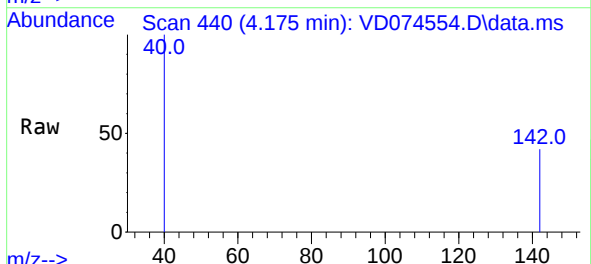


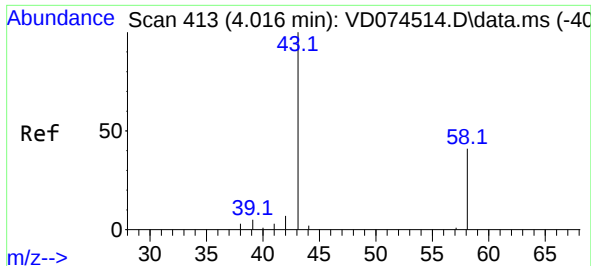

#16
Acetone
Concen: 9.729 ug/l
RT: 4.022 min Scan# 41
Delta R.T. 0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion: 43 Resp: 73
Ion Ratio Lower Upper
43 100
58 0.0 30.2 45.2#

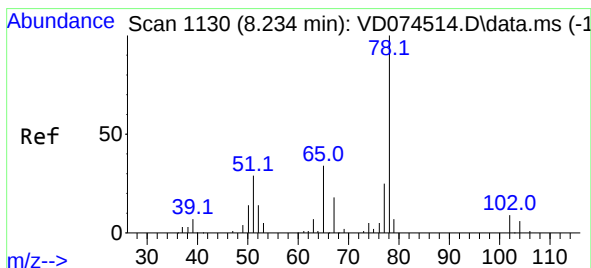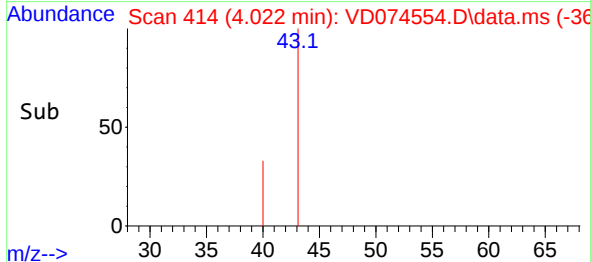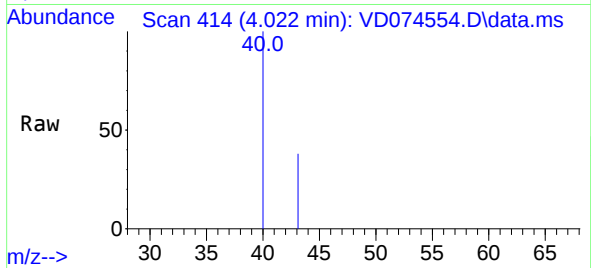

#33
1,2-Dichloroethane-d4
Concen: 106.948 ug/l
RT: 8.240 min Scan# 1131
Delta R.T. 0.012 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion: 65 Resp: 3720
Ion Ratio Lower Upper
65 100
67 61.5 0.0 110.2


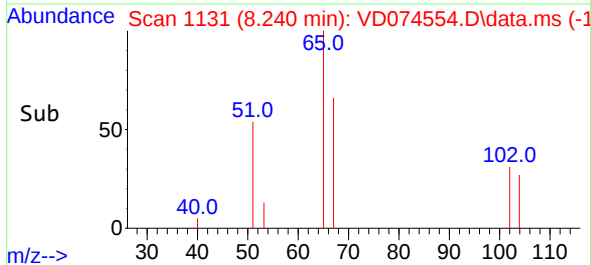

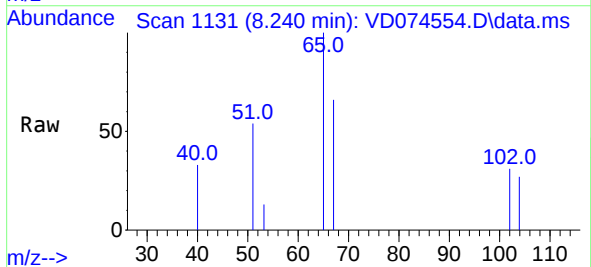


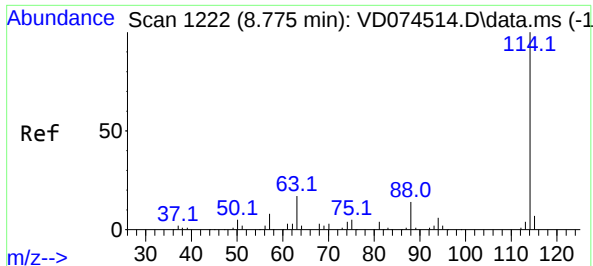

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.775 min Scan# 11
Delta R.T. 0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion:114	Resp:	7306
Ion Ratio	Lower	Upper
114	100	
63	18.3	0.0 33.2
88	12.6	0.0 28.2

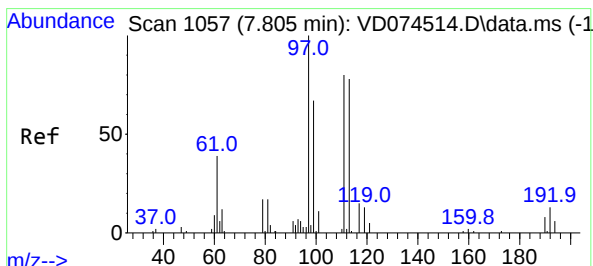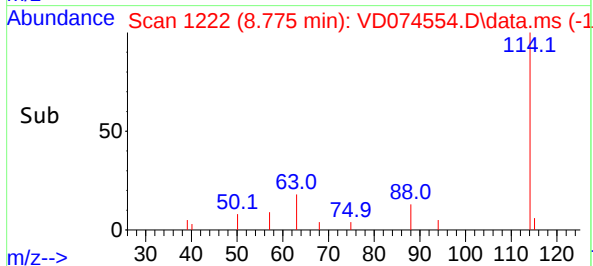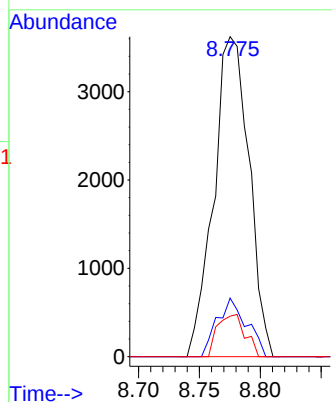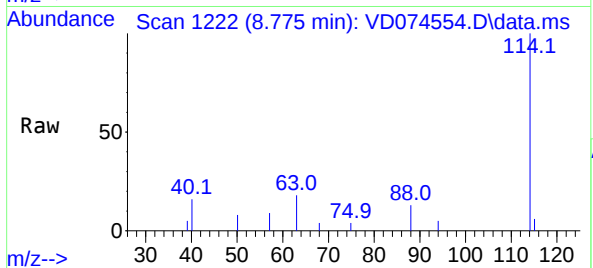

#35
Dibromofluoromethane
Concen: 85.074 ug/l
RT: 7.805 min Scan# 1057
Delta R.T. 0.001 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion:113	Resp:	3659
Ion Ratio	Lower	Upper
113	100	
111	88.5	82.3 123.5
192	12.8	16.4 24.6#

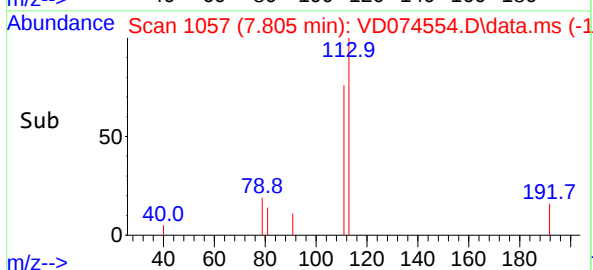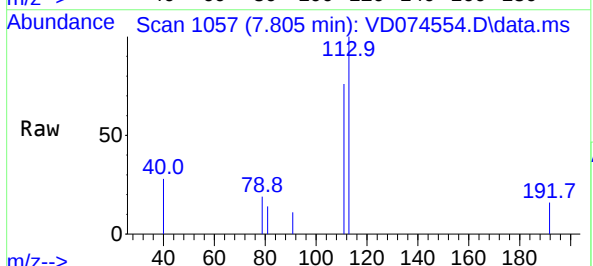

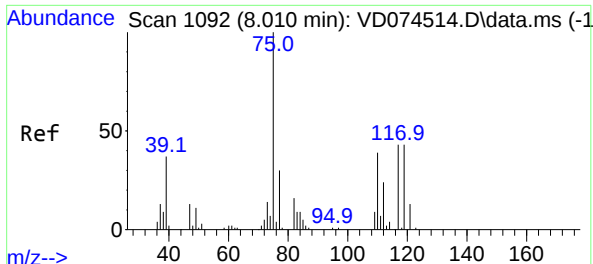

#36

1,1-Dichloropropene

Concen: 2.753 ug/l

RT: 7.875 min Scan# 1069

Delta R.T. -0.129 min

Lab File: VD074554.D

Acq: 17 Oct 2022 19:39

Instrument :

MSVOA_D

ClientSampleId :

TR-4-101422





Tgt Ion: 75 Resp: 193

Ion Ratio Lower Upper

75 100

110 0.0 19.7 59.0#

77 0.0 25.4 38.2#

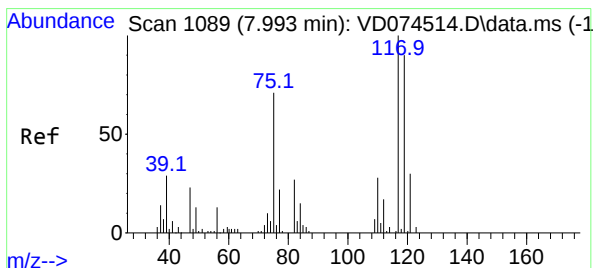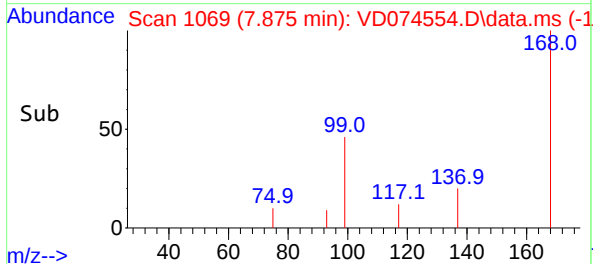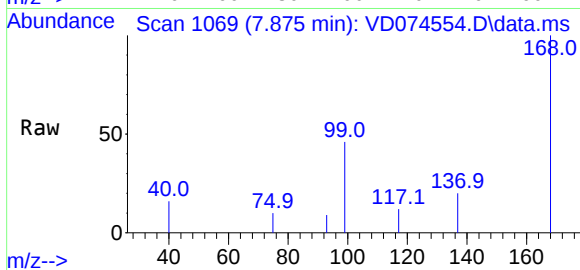

#38

Carbon Tetrachloride

Concen: 3.224 ug/l

RT: 7.875 min Scan# 1069

Delta R.T. -0.112 min

Lab File: VD074554.D

Acq: 17 Oct 2022 19:39




Tgt Ion: 117 Resp: 209


Ion Ratio Lower Upper

117 100

119 0.0 73.1 109.7#

121 0.0 25.0 37.6#


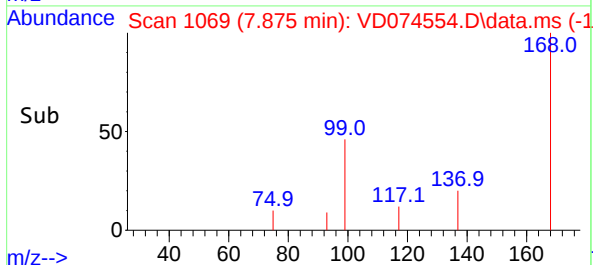
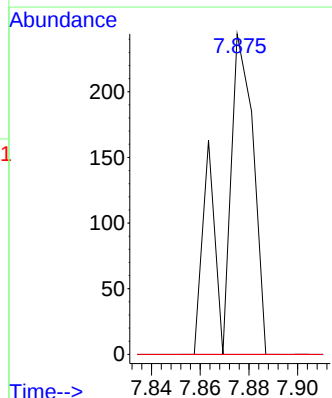
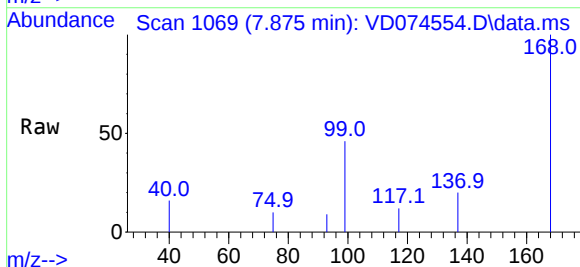


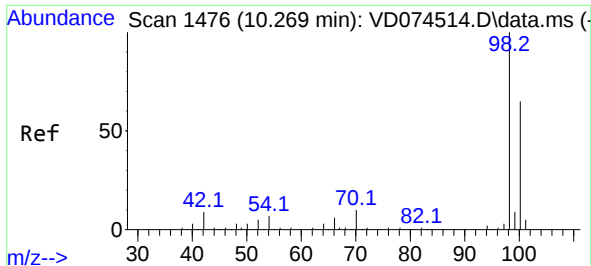

#50
Toluene-d8
Concen: 56.860 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion: 98 Resp: 9551
Ion Ratio Lower Upper
98 100
100 60.8 51.4 77.0

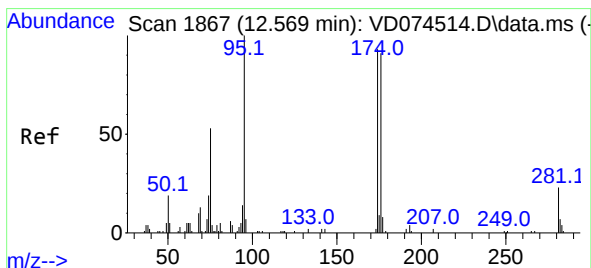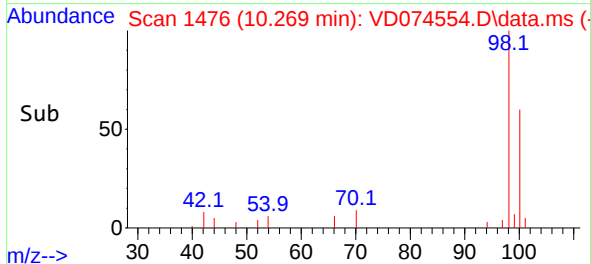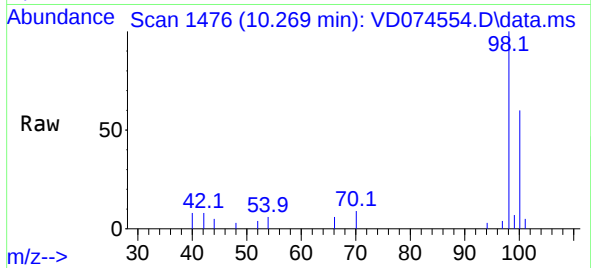

#62
4-Bromofluorobenzene
Concen: 63.585 ug/l
RT: 12.569 min Scan# 1867
Delta R.T. 0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion: 95 Resp: 3190
Ion Ratio Lower Upper
95 100
174 100.7 0.0 197.0
176 96.2 0.0 182.6


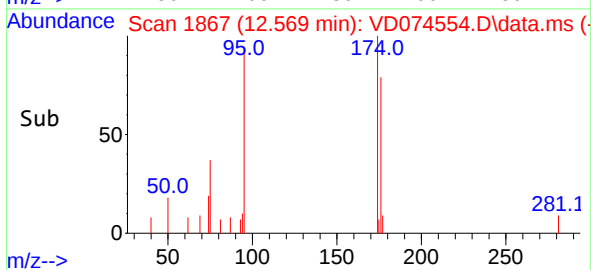

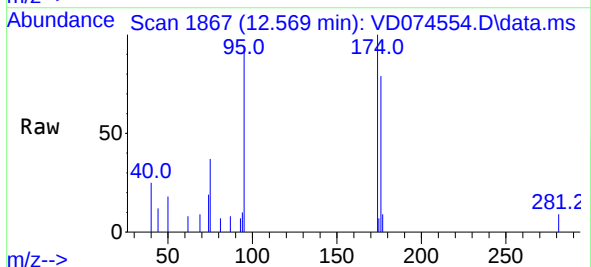


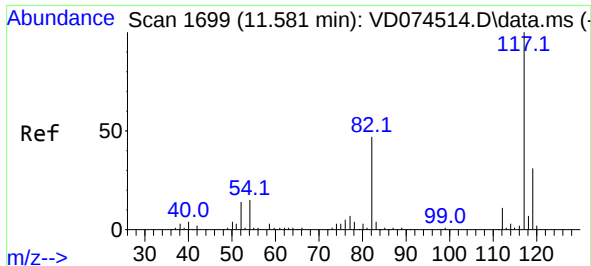

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39




Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422


Tgt Ion:	117	Resp:	7953
Ion	Ratio	Lower	Upper
117	100		
82	43.7	41.6	62.4
119	30.2	25.2	37.8

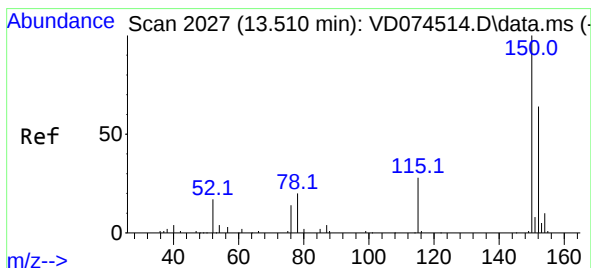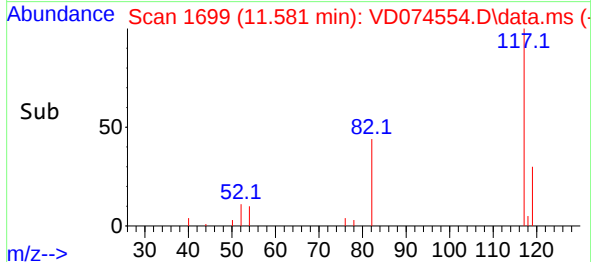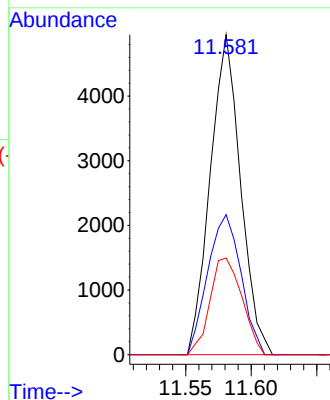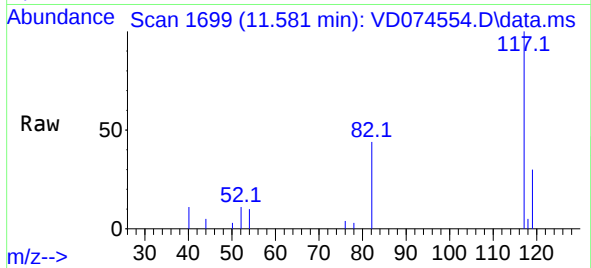

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. 0.006 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion:	152	Resp:	3625
Ion	Ratio	Lower	Upper
152	100		
115	52.1	26.8	80.4
150	162.8	0.0	348.2


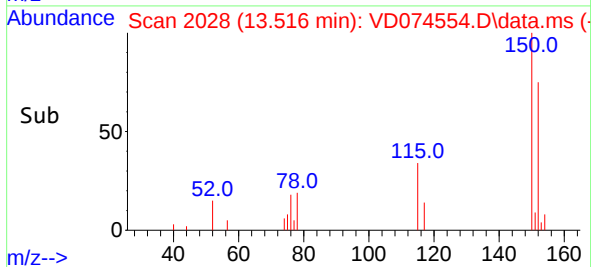
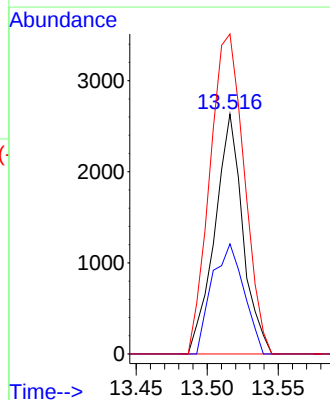
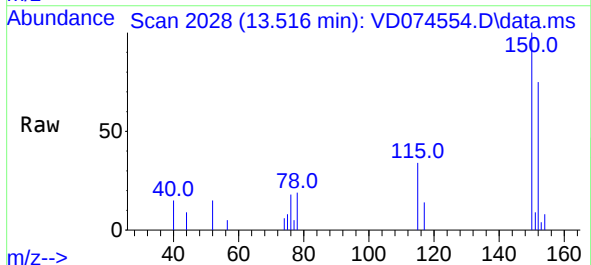


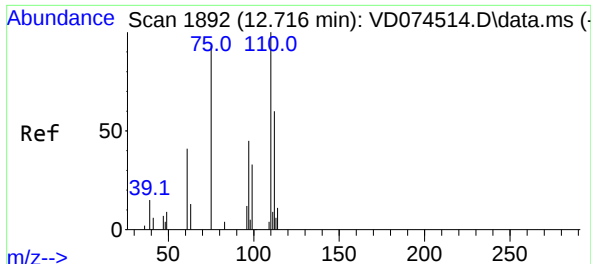

#76
1,2,3-Trichloropropane
Concen: 52.389 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.141 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Instrument :
MSVOA_D
ClientSampleId :
TR-4-101422

Tgt Ion: 75 Resp: 1623
Ion Ratio Lower Upper
75 100
77 0.0 185.8 557.5#

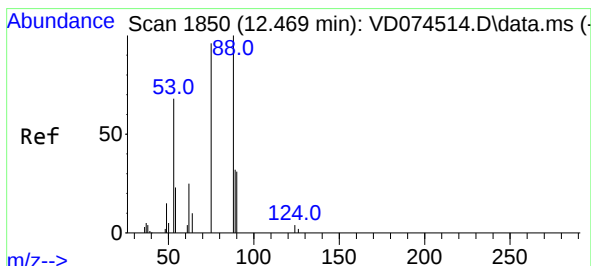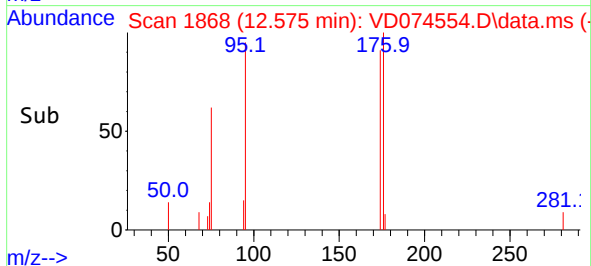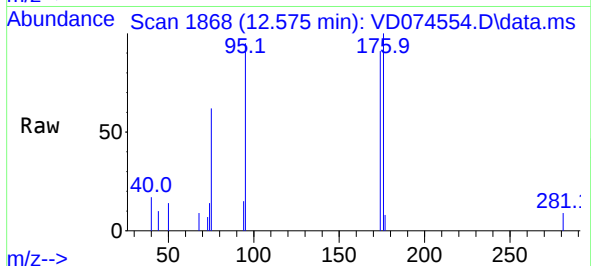

#81
trans-1,4-Dichloro-2-butene
Concen: 132.891 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.112 min
Lab File: VD074554.D
Acq: 17 Oct 2022 19:39

Tgt Ion: 75 Resp: 1623
Ion Ratio Lower Upper
75 100
53 0.0 63.8 95.6#
89 0.0 38.2 57.4#

